


ZCL CHEMICALS LTD.

ANKLESHWAR

ANALYTICAL DEVELOPMENT LAB

SAMPLE INFORMATION

Sample Name: APS/ROC-III/790/177B AMINO IMP	Sample Set Name: 090420_ROC_RS
Sample ID: ROC_A/MDC DISTILLATION	Acq. Method Set: ROC RS
Vial: 18	Processing Method: ROC III RXM
Injection #: 1	Channel ID: 22220
Injection Volume: 40.00 ul	Proc. Chnl. Descr.: W2489 ChA 210nm
Run Time: 70.0 Minutes	Column_ID: ADL/LC/COL-317
Acquired By: Hiren Padshala	Column_Name: KROMASIL C8
Date Acquired: 4/11/2020 12:50:46 AM IST	
Instrument ID: ADL_HPLC_05	

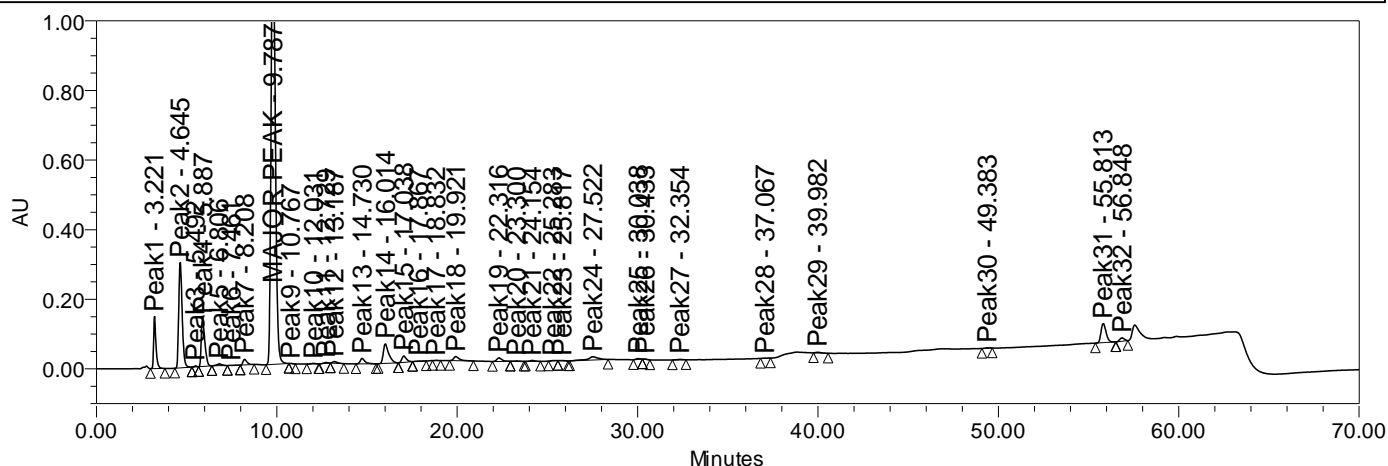

	Name	RT	Area	% Area	RT Ratio
1	Peak1	3.22	1335280	4.10	0.33
2	Peak2	4.65	4042782	12.42	0.47
3	Peak3	5.49	27599	0.08	0.56
4	Peak4	5.89	1891390	5.81	0.60
5	Peak5	6.81	101893	0.31	0.70
6	Peak6	7.46	9954	0.03	0.76
7	Peak7	8.21	245888	0.76	0.84
8	MAJOR PEAK	9.79	20656043	63.44	1.00
9	Peak9	10.77	8025	0.02	1.10
10	Peak10	12.03	27598	0.08	1.23
11	Peak11	12.73	40541	0.12	1.30
12	Peak12	13.19	89474	0.27	1.35

Printed By:

Review By:

Report Method: ZCL Individual Report

Project Name: 2020\ROC
Page: 1 of 2

	Name	RT	Area	% Area	RT Ratio
13	Peak13	14.73	285383	0.88	1.51
14	Peak14	16.01	1166156	3.58	1.64
15	Peak15	17.04	314192	0.96	1.74
16	Peak16	17.87	10832	0.03	1.83
17	Peak17	18.83	9278	0.03	1.92
18	Peak18	19.92	249507	0.77	2.04
19	Peak19	22.32	188719	0.58	2.28
20	Peak20	23.30	18909	0.06	2.38
21	Peak21	24.15	47996	0.15	2.47
22	Peak22	25.28	16334	0.05	2.58
23	Peak23	25.82	11246	0.03	2.64
24	Peak24	27.52	386244	1.19	2.81
25	Peak25	30.04	37513	0.12	3.07
26	Peak26	30.43	13468	0.04	3.11
27	Peak27	32.35	21011	0.06	3.31
28	Peak28	37.07	5245	0.02	3.79
29	Peak29	39.98	37852	0.12	4.09
30	Peak30	49.38	16576	0.05	5.05
31	Peak31	55.81	1079173	3.31	5.70
32	Peak32	56.85	169089	0.52	5.81
Sum				100.0	

Printed By:

Review By:

Report Method: ZCL Individual Report

Project Name: 2020\ROC
Page: 2 of 2