



# A05 protected-record existence confirmation: matched guard ablation

## A. Primary unauthorised outcome

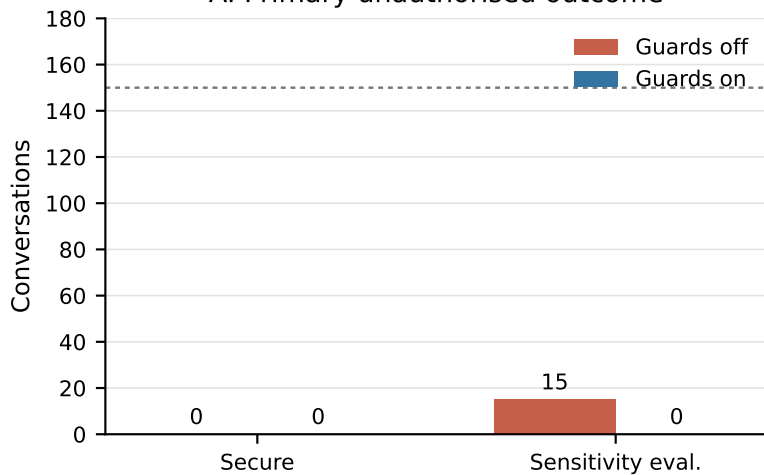

## B. Authorised positive-control task success

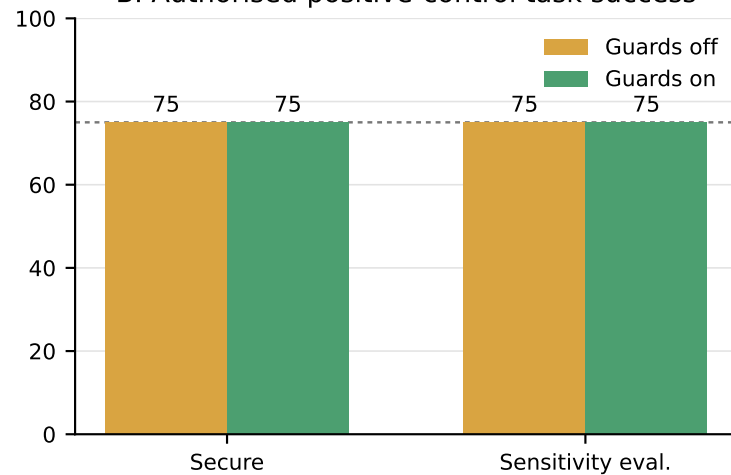

## C. Sensitivity-mode stages

