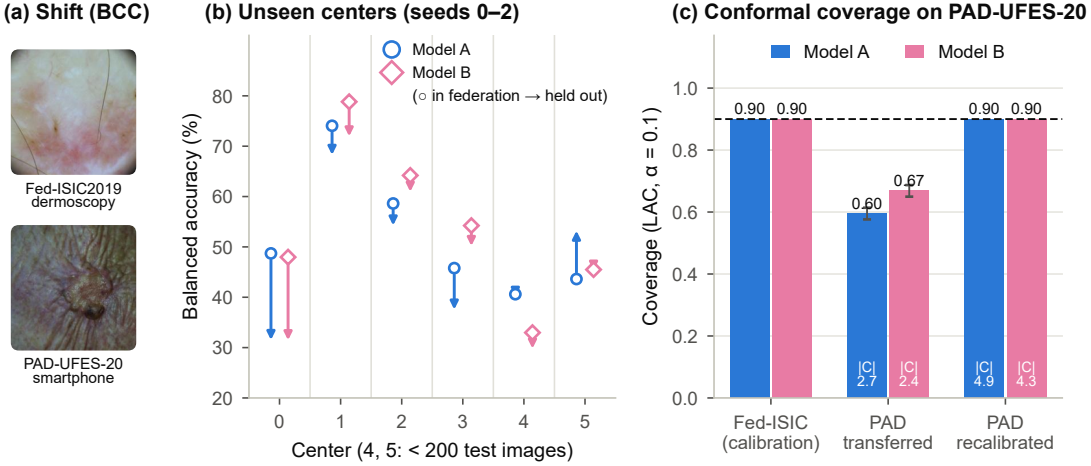

(a) Shift (BCC)
Fed-ISIC2019
dermoscopy
PAD-UFES-20
smartphone
(b) Unseen centers (seeds 0–2)
Model A
Model B
(○ in federation → held out)
Balanced accuracy (%)
80
70
60
50
40
30
20
0
1
2
3
4
5
Center (4, 5: < 200 test images)
(c) Conformal coverage on PAD-UFES-20
Model A
Model B
Coverage (LAC, α = 0.1)
1.0
0.8
0.6
0.4
0.2
0.0
0.90
0.90
0.60
0.67
0.90
0.90
|C|
2.7
|C|
2.4
|C|
4.9
|C|
4.3
Fed-ISIC
(calibration)
PAD
transferred
PAD
recalibrated
|C| = mean prediction-set size (of 6 classes); recalibrated on 50% of patients