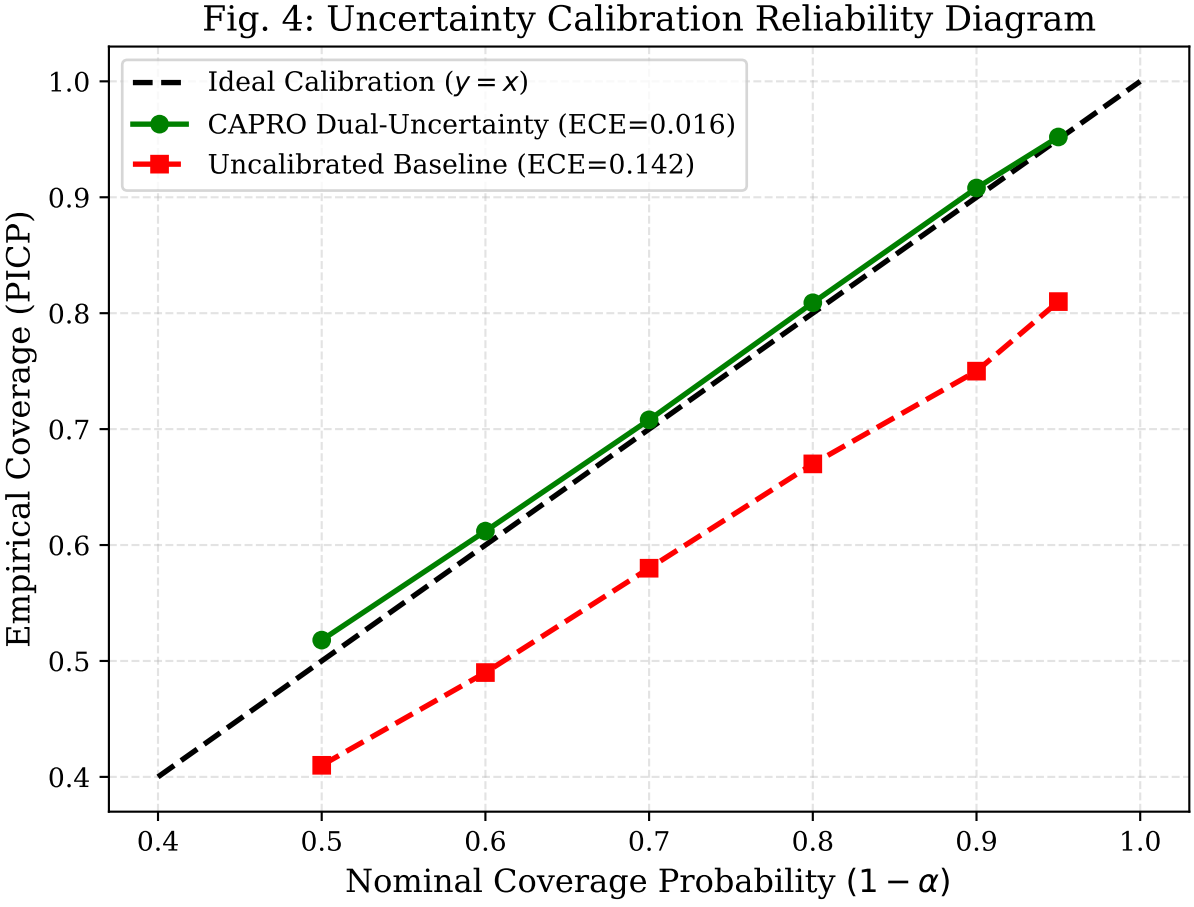
Fig. 4: Uncertainty Calibration Reliability Diagram
Ideal Calibration ($y = x$)
CAPRO Dual-Uncertainty (ECE=0.016)
Uncalibrated Baseline (ECE=0.142)
Empirical Coverage (PICP)
Nominal Coverage Probability ($1 - \alpha$)
1.0
0.9
0.8
0.7
0.6
0.5
0.4
0.4
0.5
0.6
0.7
0.8
0.9
1.0