


## Prehension trial progress and synchronization information

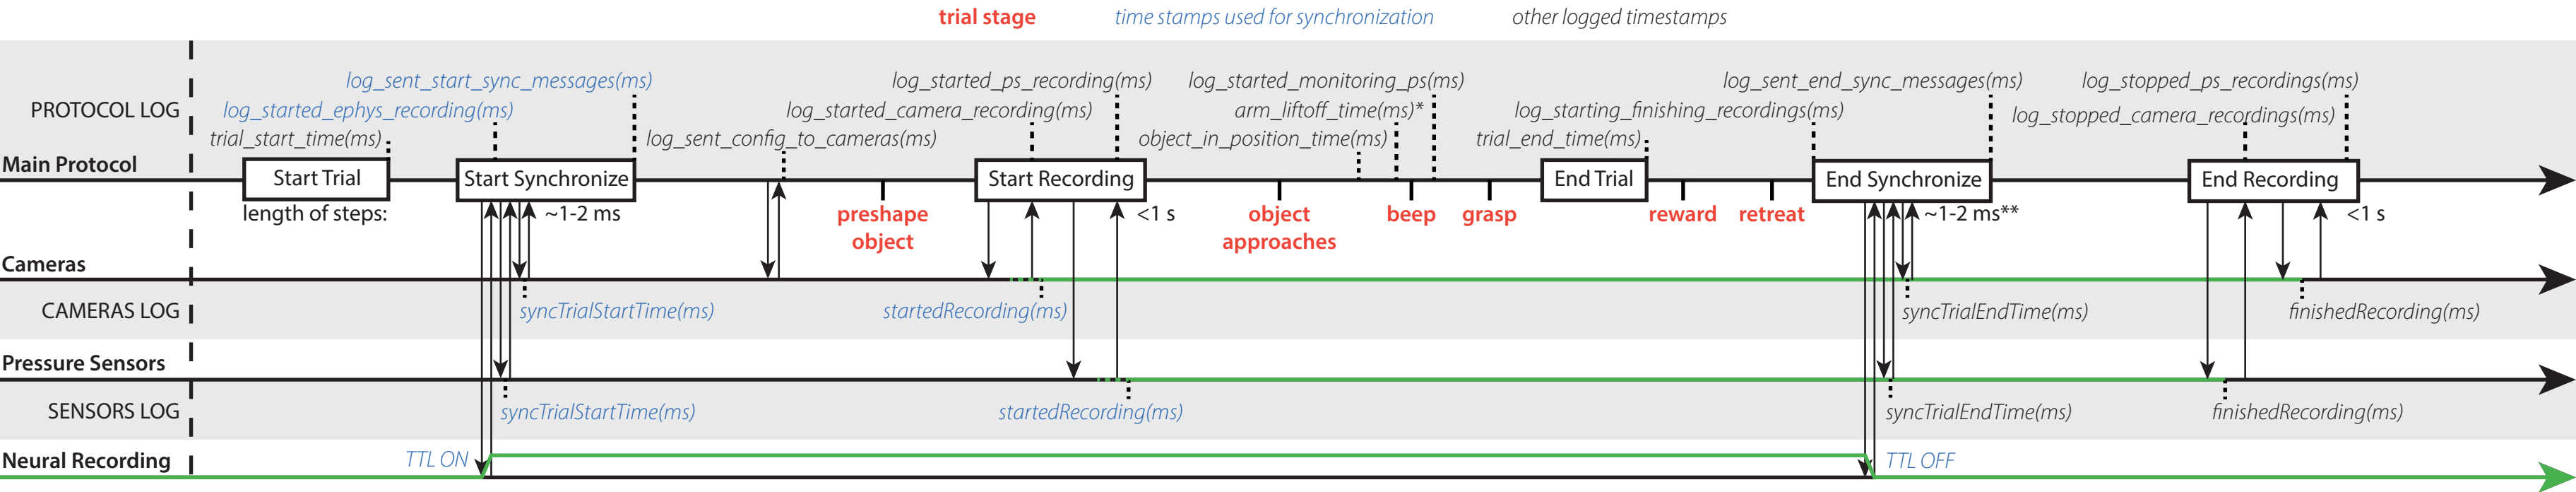

To align cameras or sensors to neural recording TTL ON pulse, add `startedRecording(ms) - syncTrialStartTime(ms)` to their internal time of the trial start.

\* Signal to start trial as shown happens after arm liftoff timestamp, however the arm liftoff is not actually tracked at this time.

\*\* Actual end synchronization time is much higher right now, closer to 200 ms because the EPHYS is controlled through a USB port on one of the computers that records from cameras.