




Manually Selected RHEED Frames and Corresponding AFM Topography

Sorted by AFM RMS Roughness - page 1


Sample 6067
RHEED
Manual selection
select_oxy.jpg

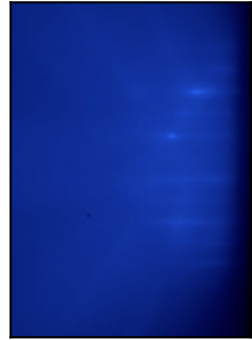



AFM
Rq = 1.274 nm
Scan: 1 x 1 um

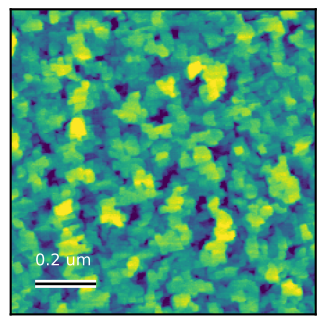


Sample 6072
RHEED
Manual selection
select_rampdown_to_250C.jpg

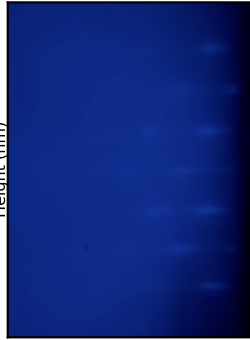



AFM
Rq = 1.470 nm
Scan: 1 x 1 um

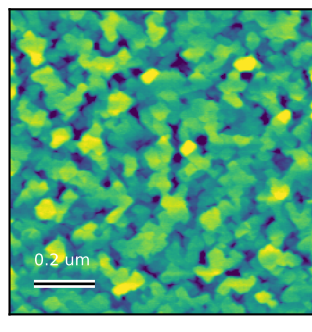


Sample 6073
RHEED
Manual selection
select_oxy.jpg

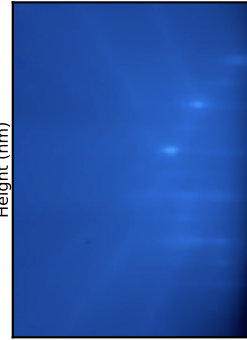



AFM
Rq = 1.517 nm
Scan: 1 x 1 um

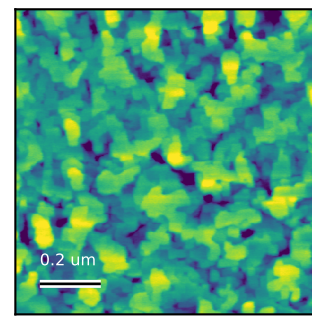


Sample 6078
RHEED
Manual selection
select_GaSb_6min.jpg

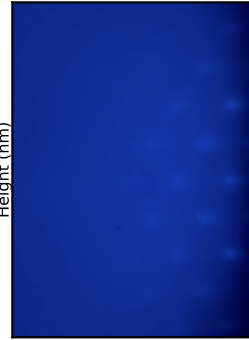



AFM
Rq = 1.638 nm
Scan: 1 x 1 um

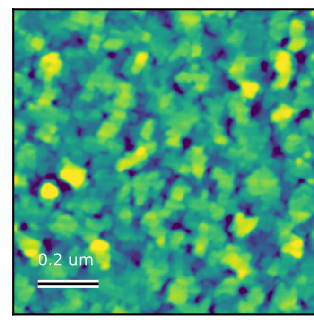


Sample 6022
RHEED
Manual selection
select_After_GaSb.jpg

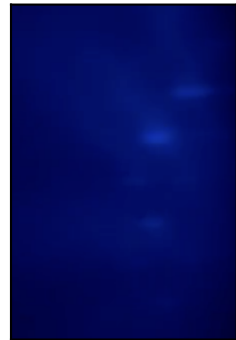



AFM
Rq = 1.649 nm
Scan: 1 x 1 um

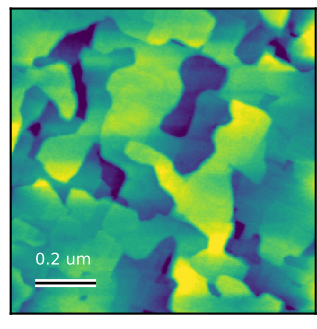


Sample 6088
RHEED
Manual selection
select_after_ramping_down_for_GaSb.jpg

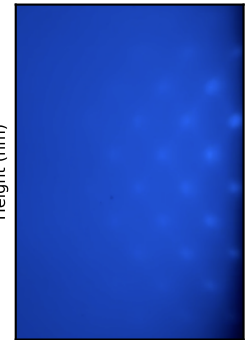



AFM
Rq = 1.832 nm
Scan: 1 x 1 um

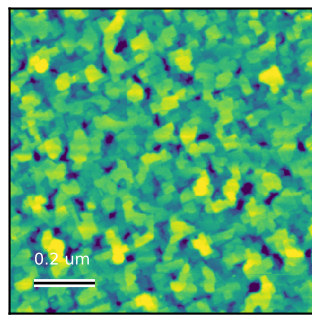


Sample 6082
RHEED
Manual selection
select_after_rampdown_to_200C.jpg

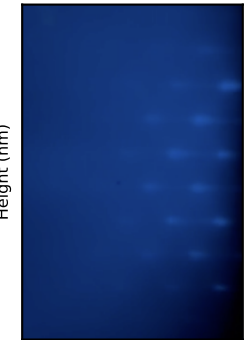



AFM
Rq = 1.864 nm
Scan: 1 x 1 um

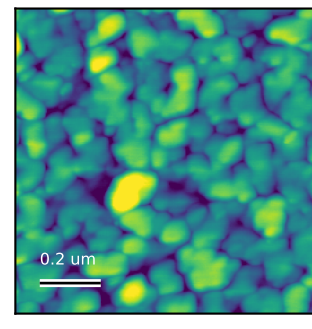


Sample 6041
RHEED
Manual selection
select_oxy.jpg

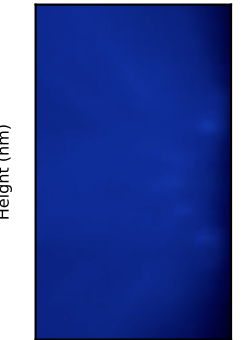



AFM
Rq = 2.019 nm
Scan: 1 x 1 um

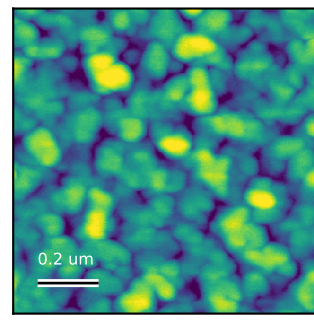


Sample 6101
RHEED
Manual selection
select_150_min_GaSb.jpg

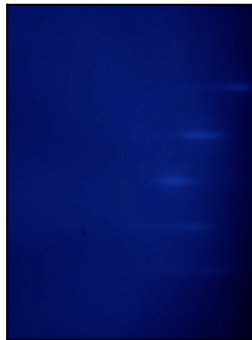



AFM
Rq = 2.127 nm
Scan: 1 x 1 um

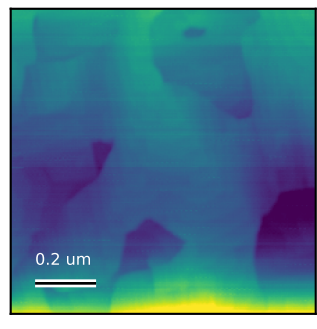

Sample 6084
RHEED
Manual selection
select_after_ramping_down_to_200C.jpg

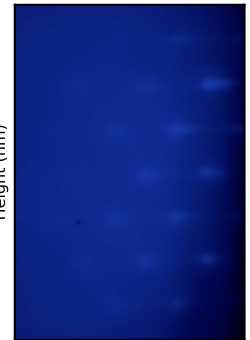



AFM
Rq = 2.473 nm
Scan: 1 x 1 um

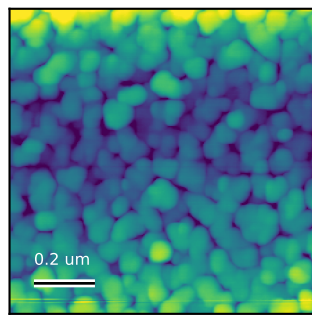


Sample 6033
RHEED
Manual selection
select_15min_of_GaSb.jpg





AFM
Rq = 2.529 nm
Scan: 1 x 1 um

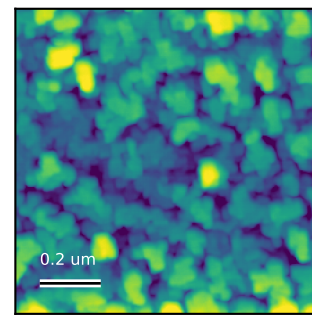


Sample 6029
RHEED
Manual selection
select_after_ramping_down_GaSb.jpg

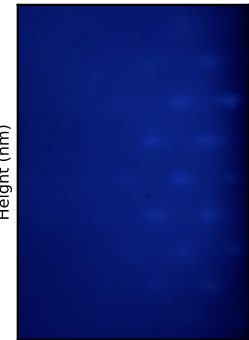



AFM
Rq = 2.561 nm
Scan: 1 x 1 um

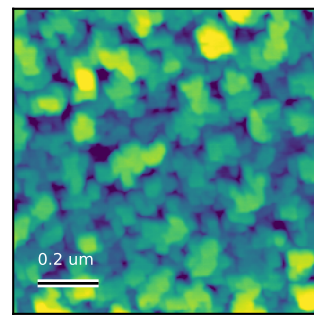


Sample 6070
RHEED
Manual selection
select_rampdown_to_300C.jpg

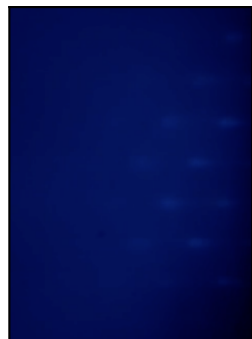



AFM
Rq = 3.047 nm
Scan: 1 x 1 um

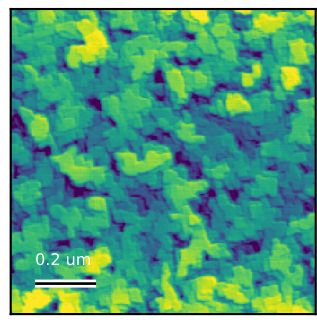


Sample 6085
RHEED
Manual selection
select_ramping_down_to_300C.jpg

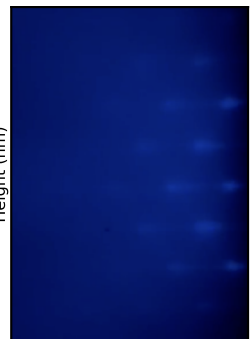



AFM
Rq = 3.095 nm
Scan: 1 x 1 um

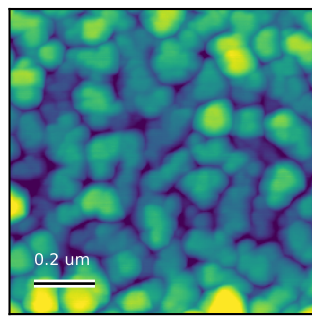


Sample 6062
RHEED
Manual selection
select_after_rampdown_to_300C.jpg

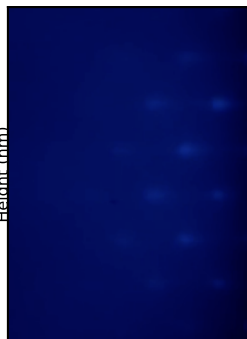

AFM
Rq = 3.177 nm
Scan: 1 x 1 um

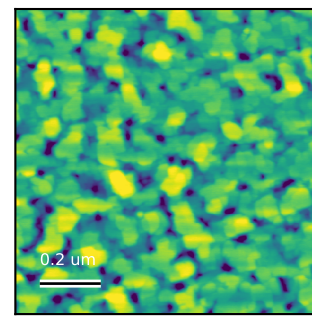

Sample 6081
RHEED
Manual selection
select_after_rampdown_for_GaSb.jpg

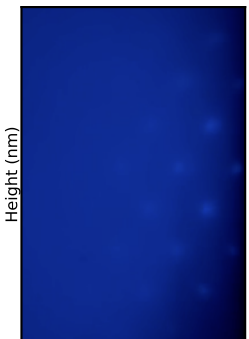

AFM
Rq = 3.181 nm
Scan: 1 x 1 um

