




Manually Selected RHEED Frames and Corresponding AFM Topography

Sorted by AFM RMS Roughness - page 2


Sample 6056
RHEED
Manual selection
select_after_rampdown_to_200C.jpg

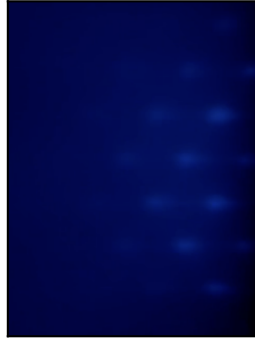



AFM
Rq = 3.225 nm
Scan: 1 x 1 um

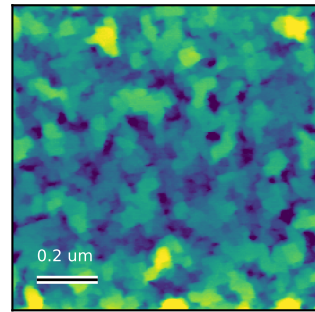


Sample 6048
RHEED
Manual selection
select_after_rampdown.jpg

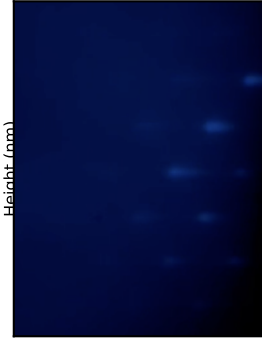



AFM
Rq = 3.227 nm
Scan: 1 x 1 um

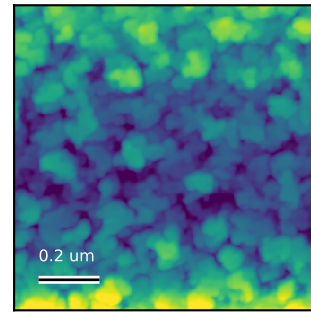


Sample 6094
RHEED
Manual selection
select_GaSb_5min.jpg

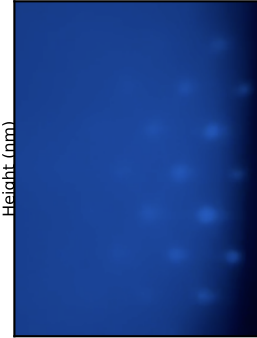



AFM
Rq = 4.127 nm
Scan: 1 x 1 um

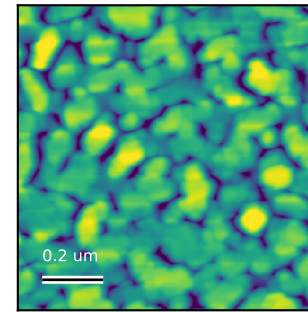


Sample 6090
RHEED
Manual selection
select_rampdown_to_200C.jpg

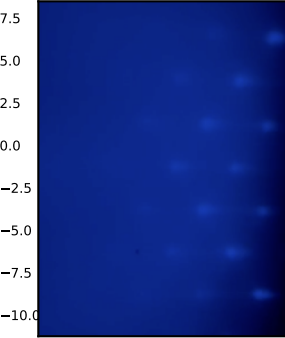



AFM
Rq = 4.685 nm
Scan: 1 x 1 um

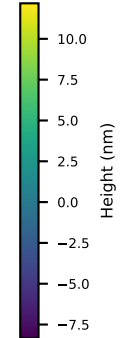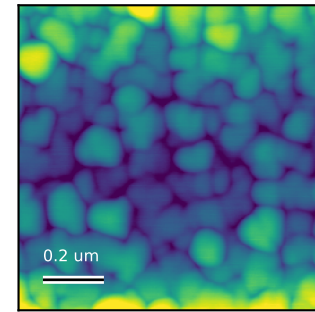


Sample 6047
RHEED
Manual selection
select_after_rampdown_to_200C.jpg

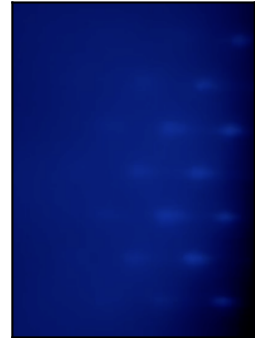



AFM
Rq = 4.693 nm
Scan: 1 x 1 um

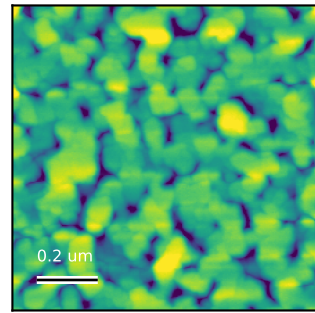

Sample 6080
RHEED
Manual selection
select_after_rampdown_to_200C.jpg

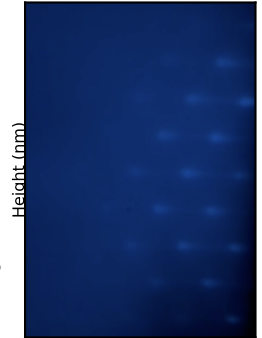



AFM
Rq = 5.159 nm
Scan: 1 x 1 um

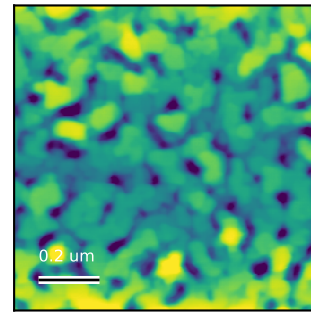


Sample 6057
RHEED
Manual selection
select_GaSb_2min.jpg





AFM
Rq = 5.337 nm
Scan: 1 x 1 um

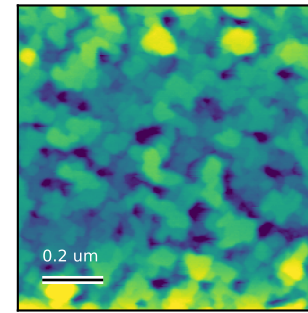


Sample 6063
RHEED
Manual selection
select_rampdown_to_300C.jpg

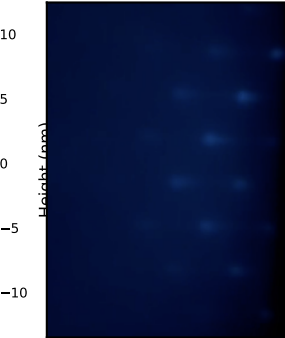



AFM
Rq = 6.004 nm
Scan: 1 x 1 um

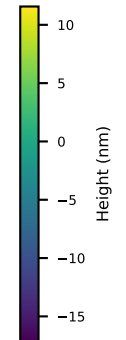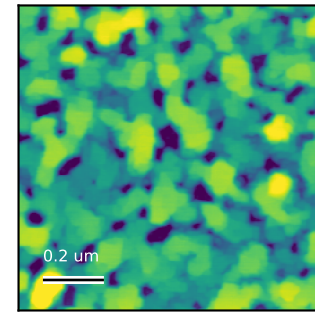


Sample 6028
RHEED
Manual selection
select_GaSb.jpg

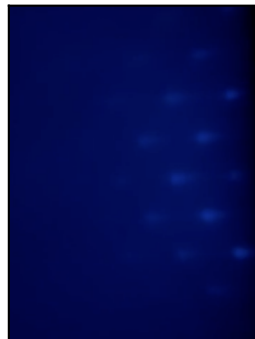



AFM
Rq = 6.073 nm
Scan: 1 x 1 um

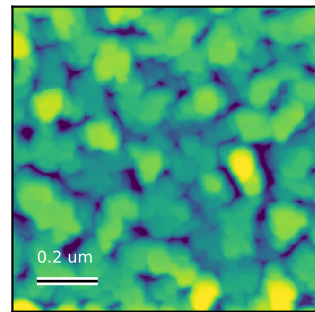


Sample 6043
RHEED
Manual selection
select_after_ramping_to_GaSb.jpg

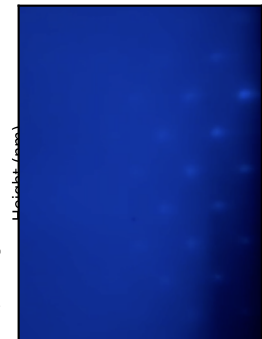



AFM
Rq = 7.372 nm
Scan: 1.02 x 1.02 um

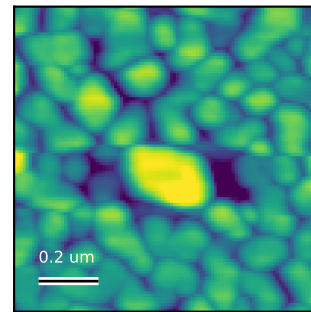


Sample 6097
RHEED
Manual selection
select_2min_GaSb.jpg

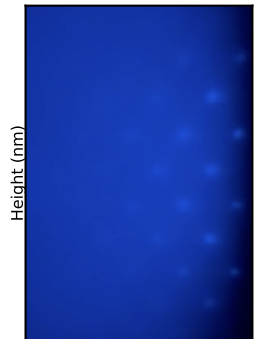



AFM
Rq = 9.224 nm
Scan: 1 x 1 um

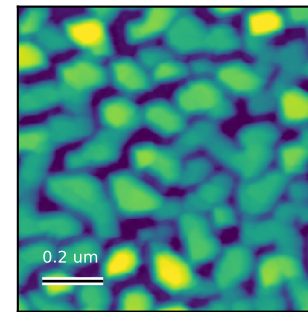


Sample 6095
RHEED
Manual selection
select_rampdown_to_250C.jpg

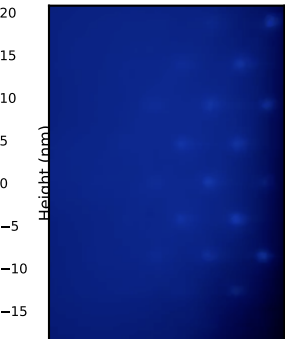



AFM
Rq = 9.867 nm
Scan: 1 x 1 um

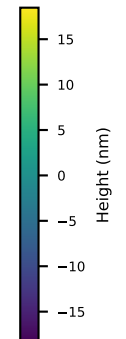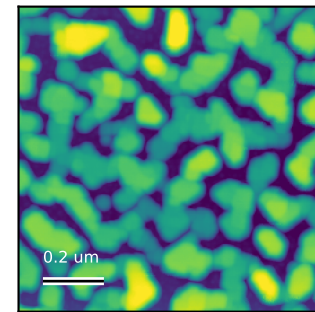


Sample 6023
RHEED
Manual selection
select_after_ramping_down.jpg

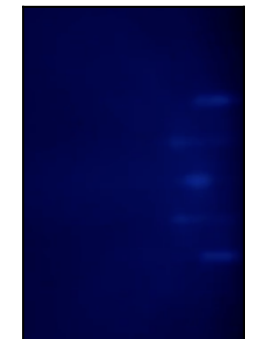

AFM
Rq = 10.290 nm
Scan: 1 x 1 um

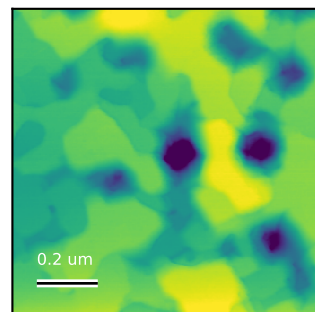

Sample 6099
RHEED
Manual selection
select_ramping_to_650C.jpg

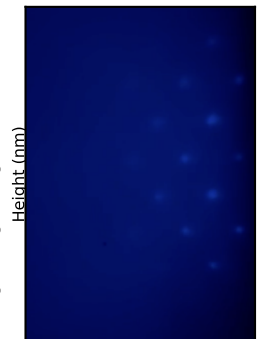

AFM
Rq = 10.321 nm
Scan: 1 x 1 um

