


Validation condition differentiation at a shared physical height scale

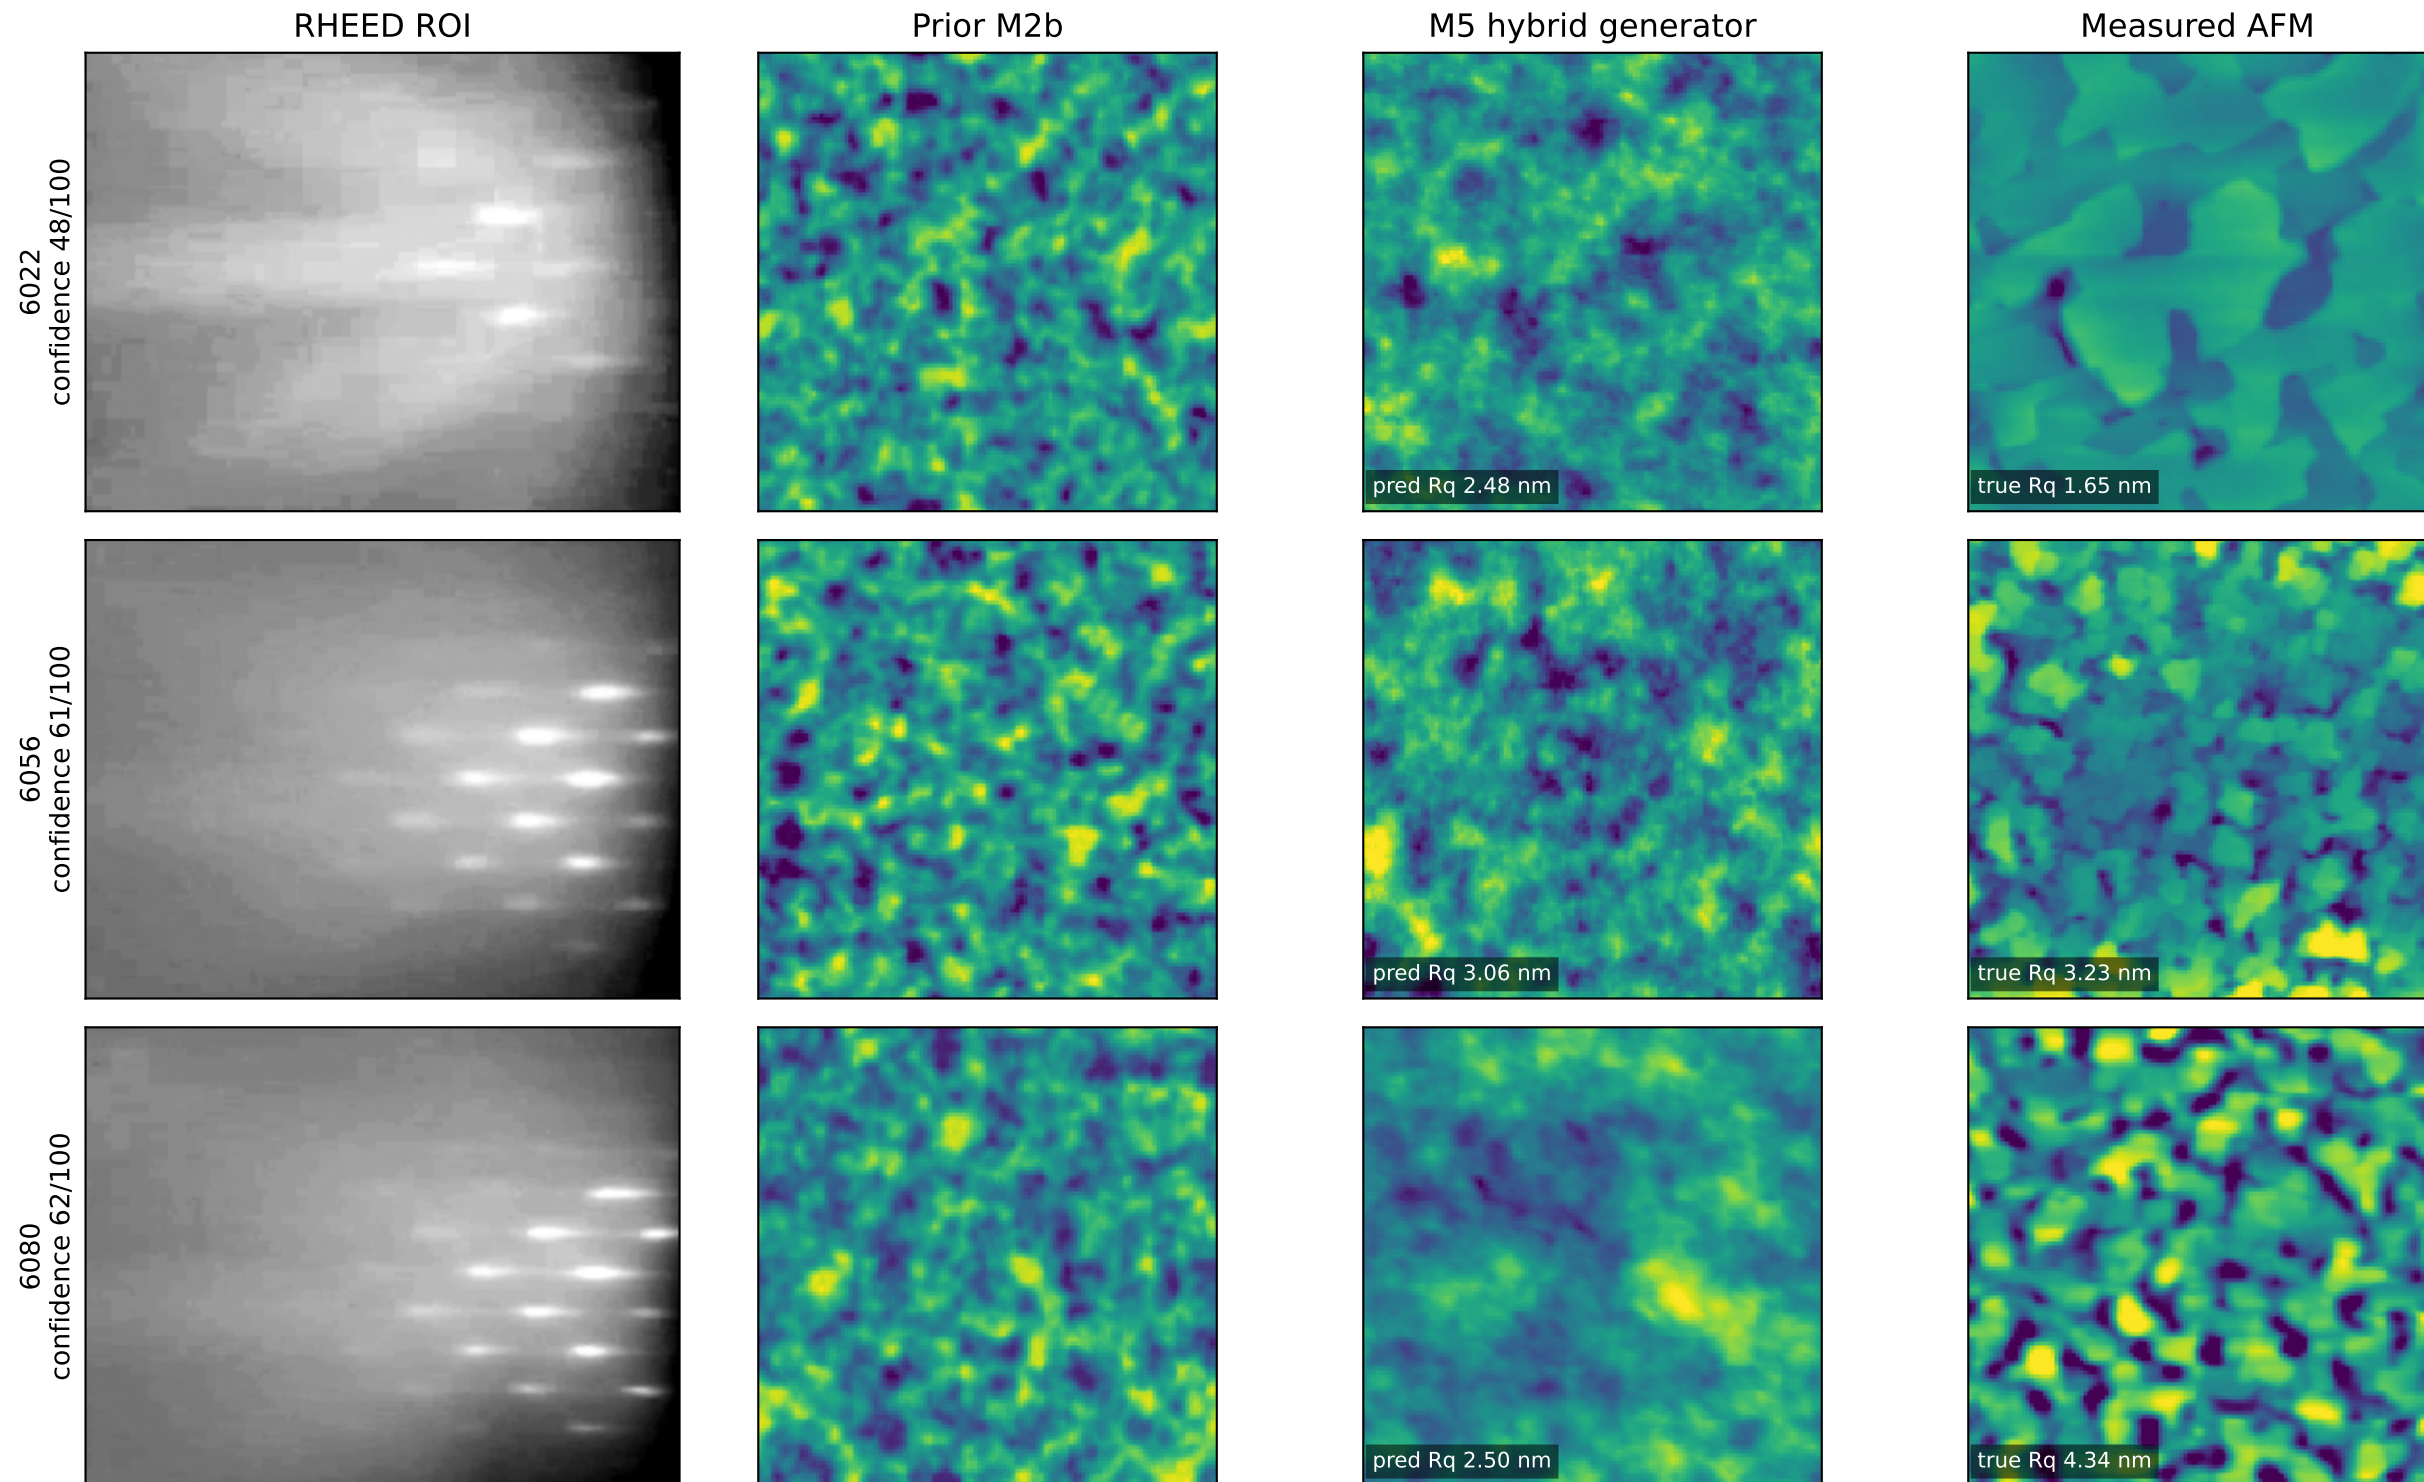

All AFM panels share ± 8.7 nm. No row is shown in unit-Rq scale; amplitude differences remain visible.