
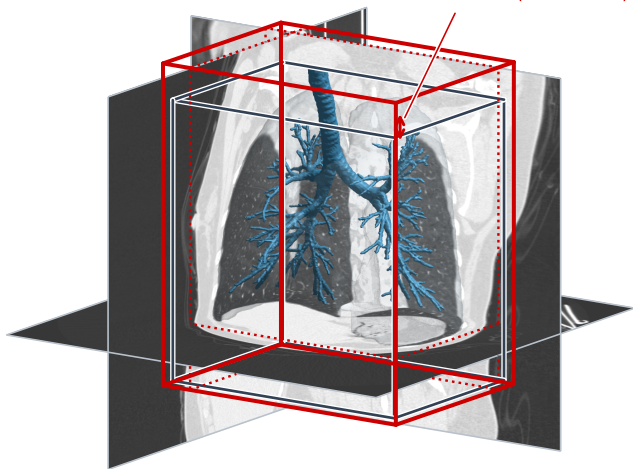


aATM_016: acquisition volume, $512 \times 512 \times 714$ voxels

superior extension:
+71 voxels available (+120 max)

**b**

staged input: outside the ROI set to 0 HU, 24.7% retained

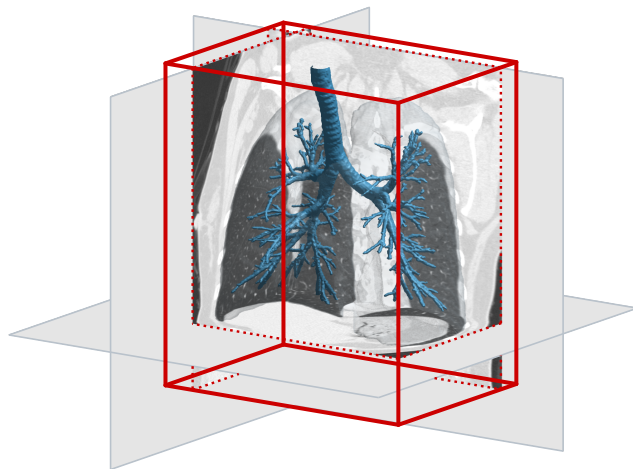

— reference airway tree

— lung-mask bounding box

— lung mask

— retained ROI (+8 voxels, +120 superior)

..... ROI where it cuts each plane