

Sample Name: PureH2


```

=====
Acq. Operator   : KM
Acq. Instrument : Instrument 1                Location : Vial 1
Injection Date  : 10/2/2026 18:07:42
                                           Inj Volume : Manually

Acq. Method     : C:\CHEM32\1\METHODS\BIOGAS-H2\CHULASAMPLE.M
Last changed    : 10/2/2026 18:06:49 by KM
                  (modified after loading)

Analysis Method : C:\CHEM32\1\METHODS\BIOGAS-H2\CHULASAMPLE.M
Last changed    : 10/2/2026 19:44:20 by KM
                  (modified after loading)

```

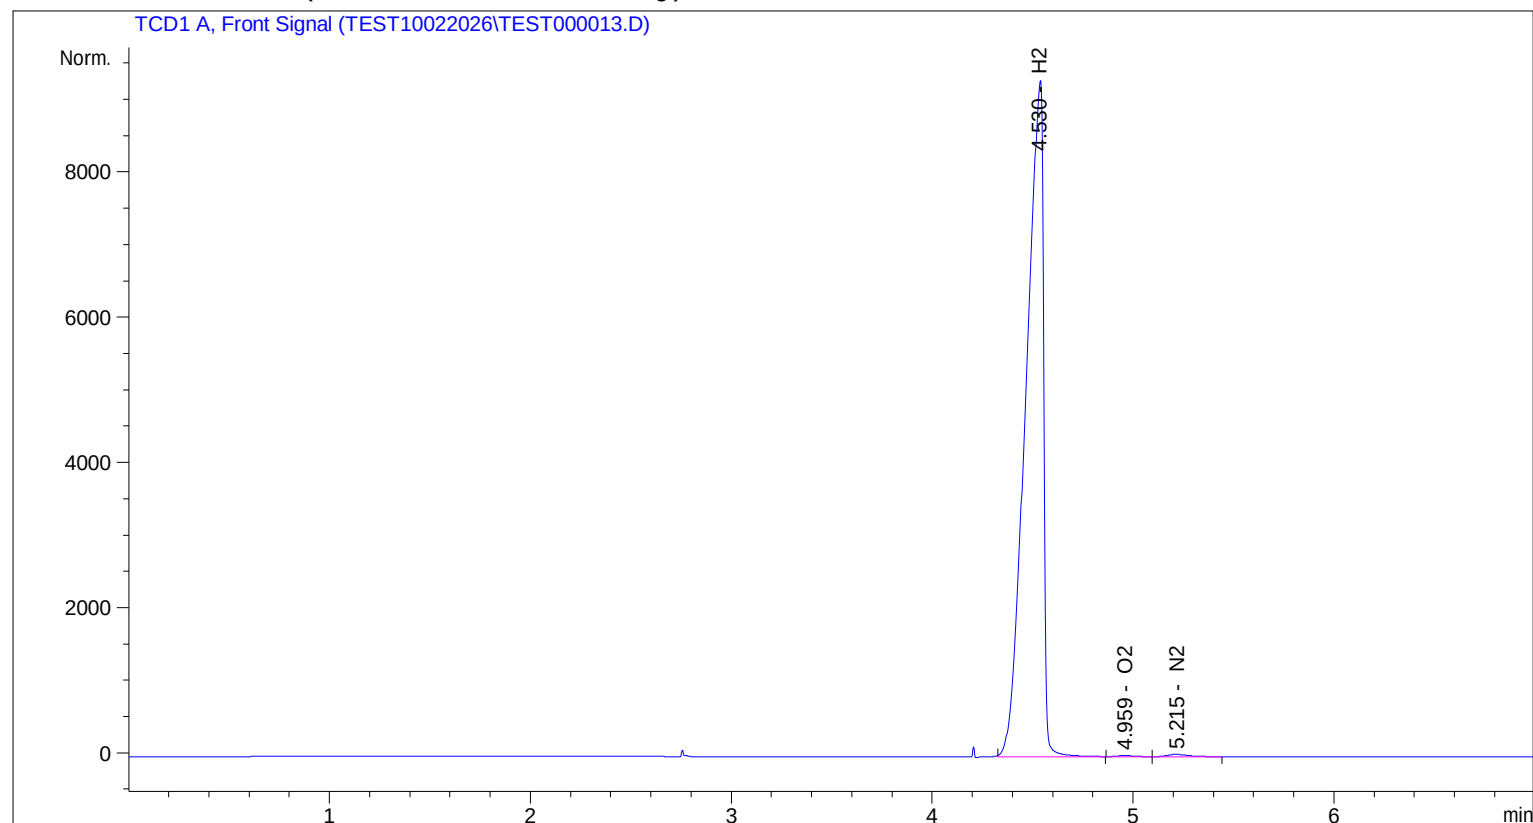

```

=====
                        Area Percent Report
=====

```

```

Sorted By           :      Signal
Calib. Data Modified :      10 February 2026 19:44:20
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: TCD1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [25 µV*s]	Area %	Name
1	3.577		0.0000	0.00000	0.00000	CO2
2	4.530	BB	0.0989	5.65682e4	99.38296	H2
3	4.959	BV	0.0956	104.50076	0.18359	O2
4	5.215	VB	0.1133	246.71411	0.43344	N2

Totals : 5.69195e4

Sample Name: PureH2

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====
*** End of Report ***