


Sample Name: PureH2

```
=====
Acq. Operator   : KM
Acq. Instrument : Instrument 1                Location : Vial 1
Injection Date  : 10/2/2026 17:50:17
                                           Inj Volume : Manually

Acq. Method     : C:\CHEM32\1\METHODS\BIOGAS-H2\CHULASAMPLE.M
Last changed    : 10/2/2026 17:48:33 by KM
                  (modified after loading)

Analysis Method : C:\CHEM32\1\METHODS\BIOGAS-H2\CHULASAMPLE.M
Last changed    : 10/2/2026 19:44:20 by KM
                  (modified after loading)
=====
```

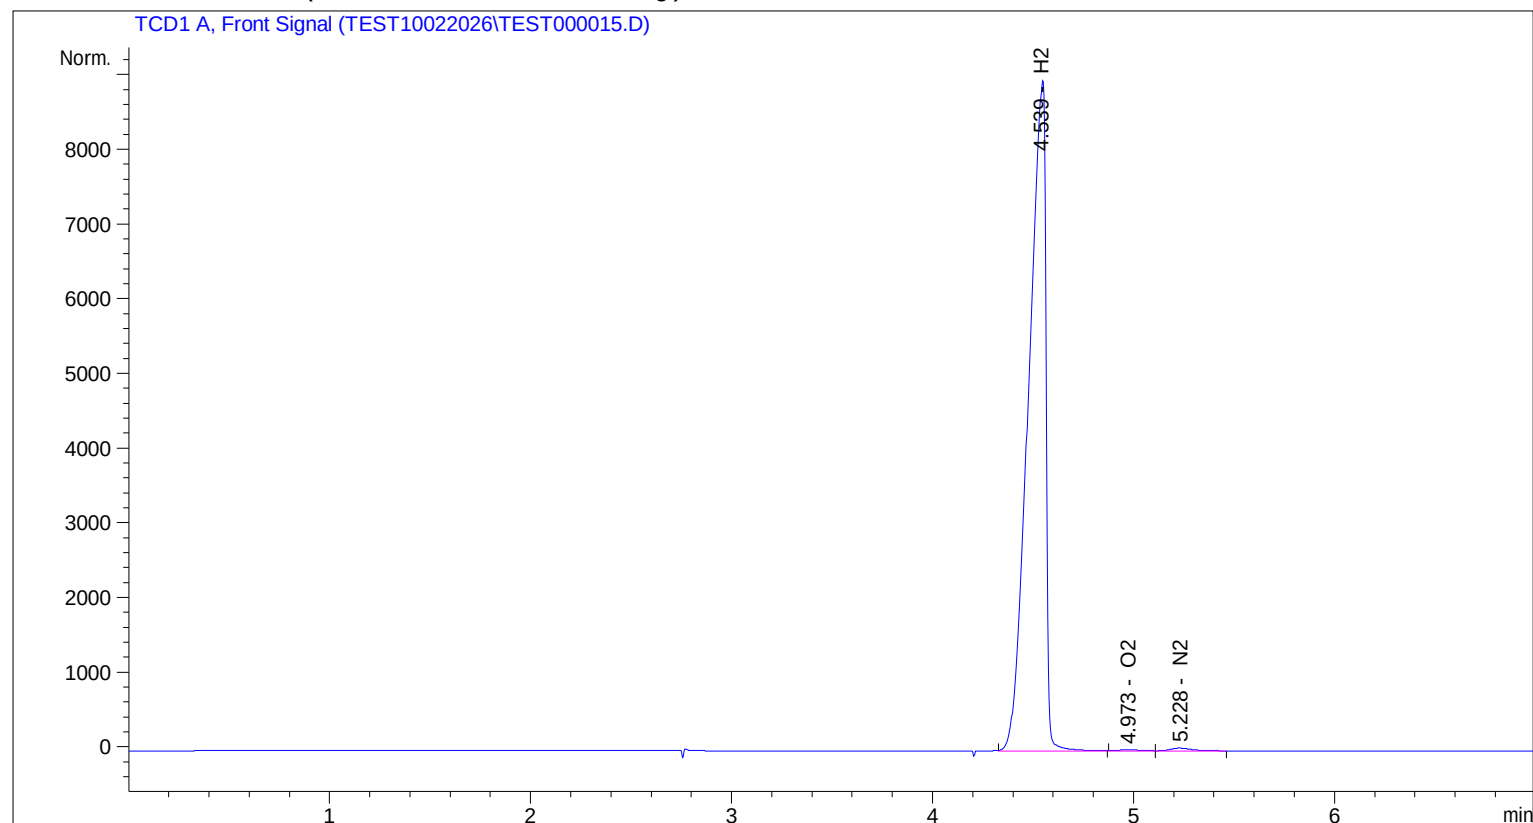

```
=====
                        Area Percent Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      10 February 2026 19:44:20
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: TCD1 A, Front Signal

Peak #	RetTime [min]	Type	Width [min]	Area [25 μ V*s]	Area %	Name
1	3.577		0.0000	0.00000	0.00000	CO2
2	4.539	BB	0.0939	5.32780e4	99.27501	H2
3	4.973	BV	0.0954	113.65521	0.21178	O2
4	5.228	VB	0.1137	275.42816	0.51322	N2

Totals : 5.36671e4

Sample Name: PureH2

1 Warnings or Errors :

Warning : Calibrated compound(s) not found

=====
*** End of Report ***