
ISO 230-2 v3: the averaging windows ran into the next move


Record windows taken from the board log through the fitted clock, drawn on the interferometer trace. The capture is sound; the window placement is not.
ISO230-2_v3.csv · terminal_20261021_183115.log · 240 ISO stops, 24 targets × 2 directions × 5 runs · motion gate 0.10 µm/ms held 20 ms

Every window closes 38 ms after the stage has left the target — 23 µm of travel, signed with the pass — which shifts B by +1.25 µm and turns −1.60 µm into −0.37 µm.


a one hold, as the published evaluation saw it (up pass)

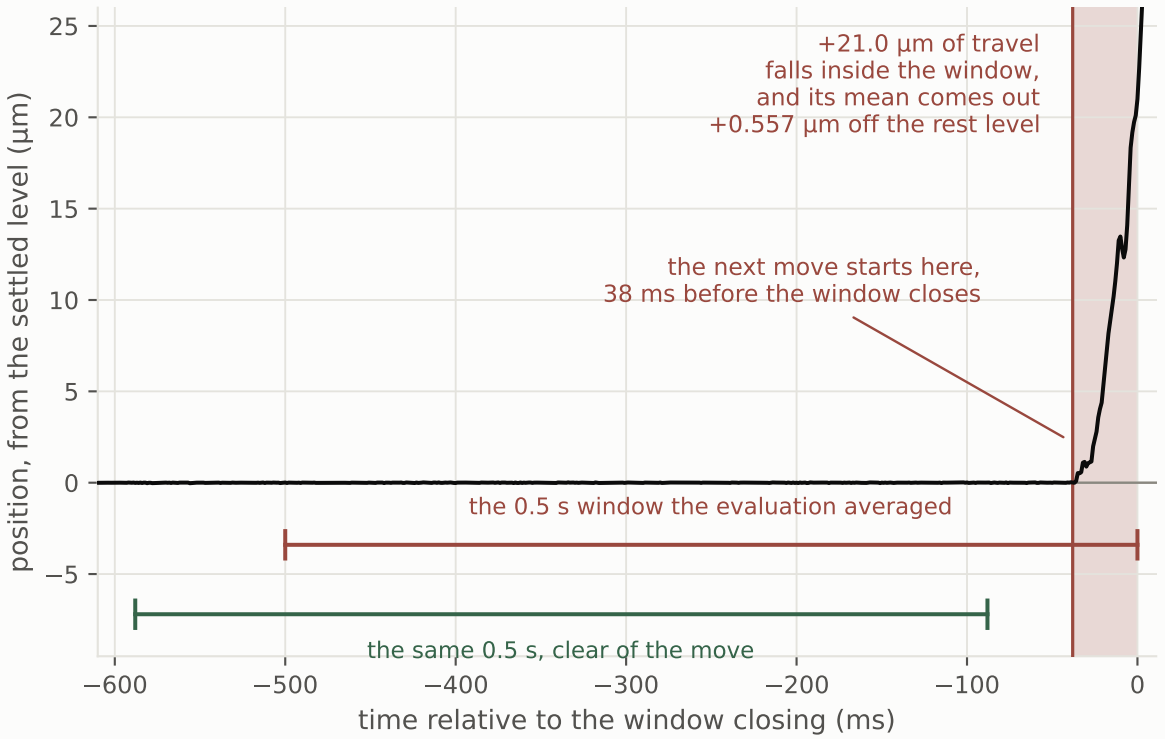

b all 240 windows, levelled on their own rest

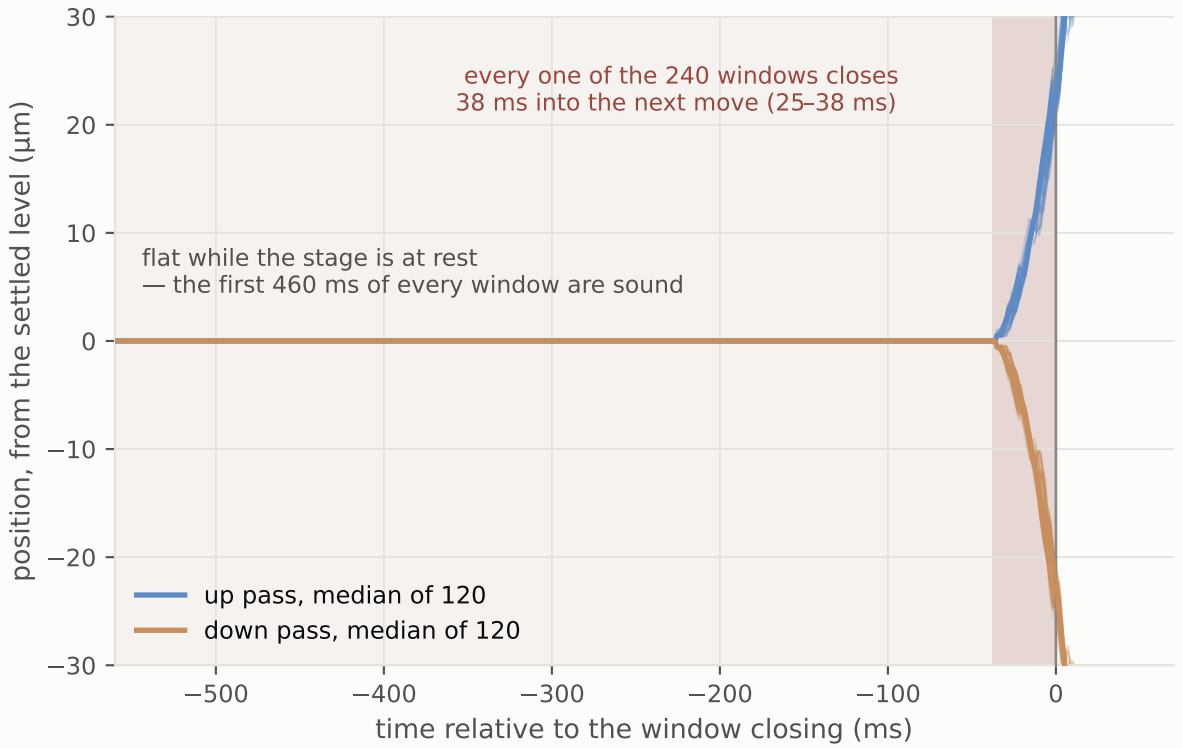

c the bias on each of the 240 window means

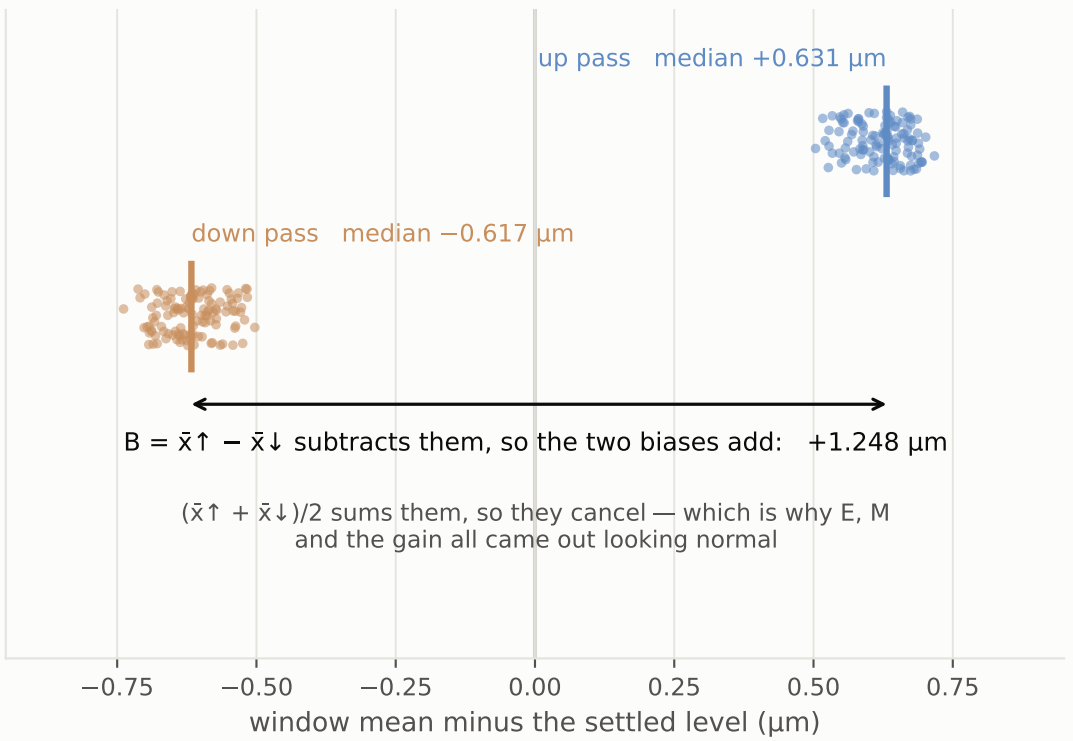

d the cliff the published value sits on

