PharmaDrishti GlucoTwin — Type 2 Diabetes Digital Twin Architecture

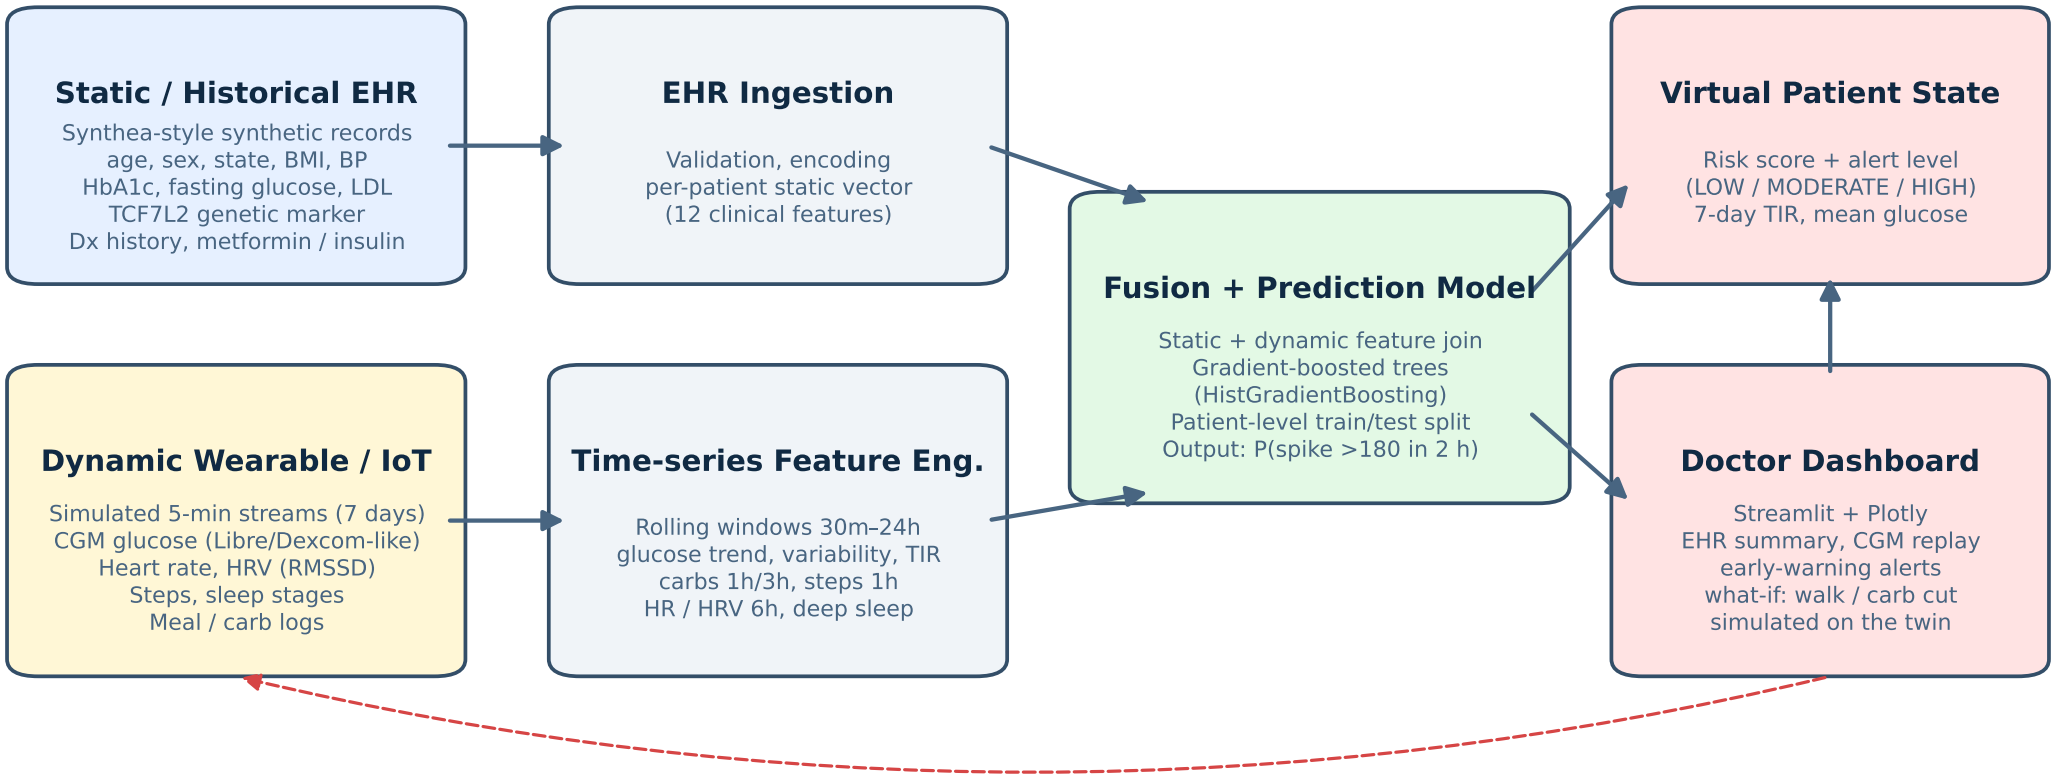

Feedback loop: new CGM/wearable readings continuously update the twin (every 5 min)

Held-out patients: ROC-AUC 0.96 · recall 0.876 · PR-AUC 0.803 | Privacy: 100% synthetic data (DPDP / HIPAA safe)