

25 mm/s, 10 mm/mV

Heart rate:	69
P duration:	- ms
PR:	- ms
QRS dur.:	161 ms
T peak:	332 ms
QT:	460 ms
QTc:	495 ms
RR Interval:	864 ms

normal PathECG

QRS:	23 %
ST:	0 %
T-wave:	0 %

normal WaveECG



QRS:	27 %
ST:	0 %
T-wave:	0 %




Look on next pages for more details

Patient ID: CienECG examples - ECG : LBBB female 82 id-15906.ecg

Report number: 0001000100000131

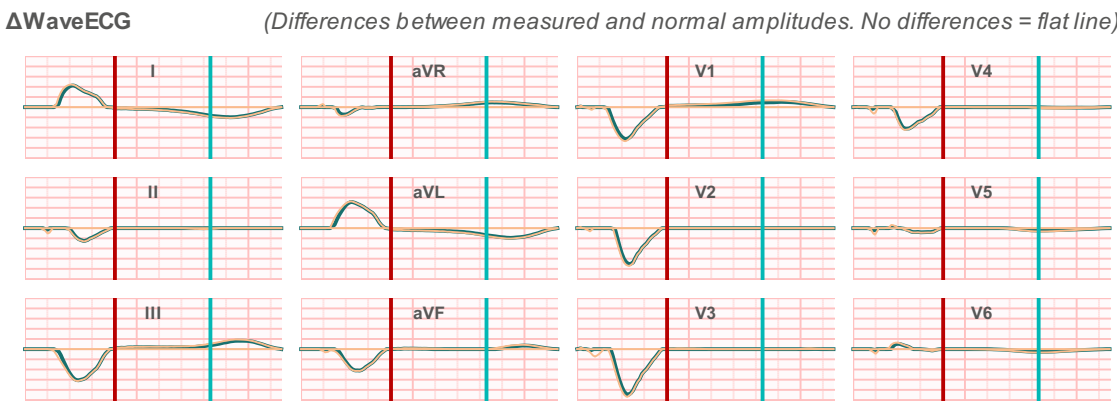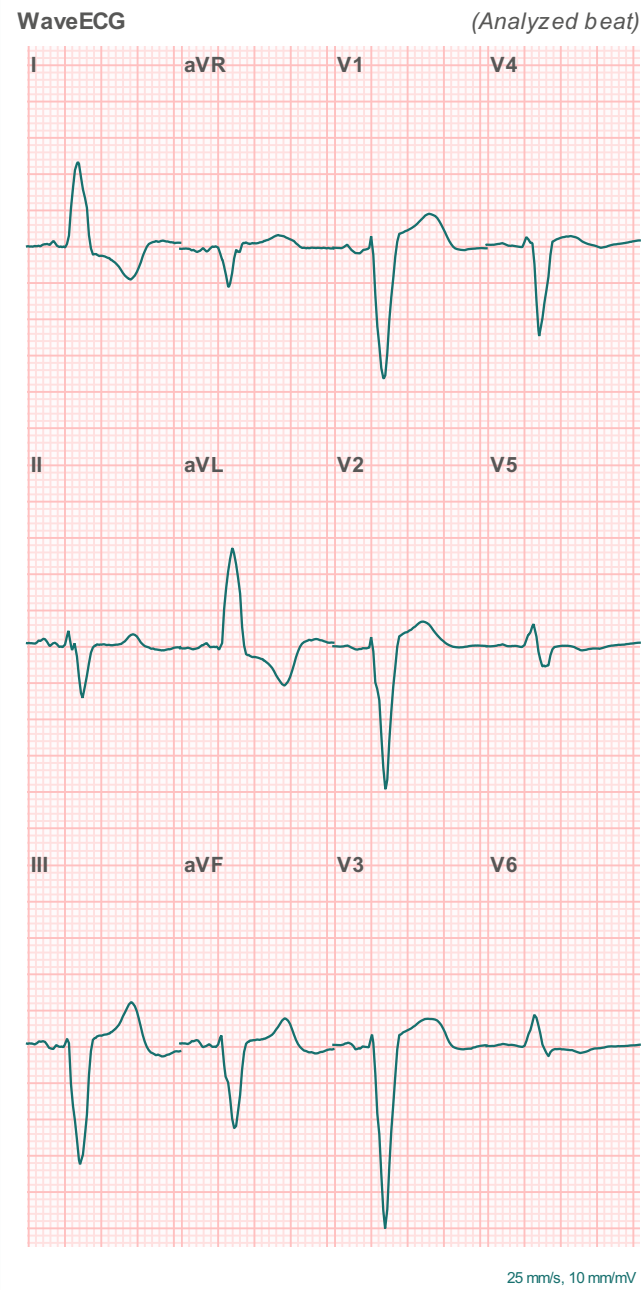

normal WaveECG	
QRS:	27 %
ST:	0 %
T-wave:	0 %

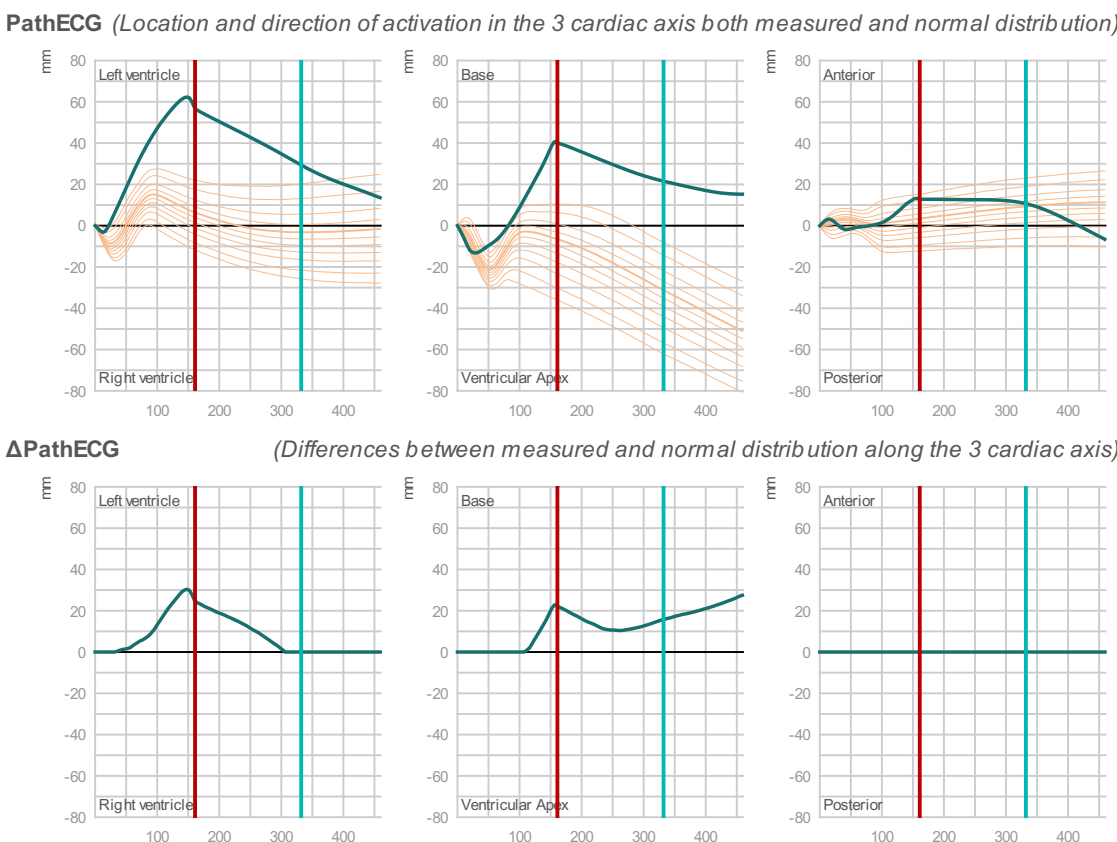

normal PathECG	
QRS:	23 %
ST:	0 %
T-wave:	0 %

Patient ID: CienECG examples - ECG : LBBB female 82 id-15906.ecg

Report number: 0001000100000131

CineECG Normal Compare

(CineECG comparison: in normal range (5-95%) green, borderzone orange, outside normal range red)

4 chamber



RAO




LAO




CineECG Locations

(CineECG trajectory related to the cardiac anatomy)



4 chamber



RAO



LAO



This version of CineECG is a research only beta version. CineECG is a brand of ECG Excellence BV, The Netherlands. CineECG analysis is based on patented technology (Patents pending). CineECG does not provide a diagnostic analysis. CineECG shows: a) the deviation between normal expected CineECG patterns and the CineECG derived from 12 lead ECG data; b) the deviation between normal ECG amplitudes and the median beat ECG. CineECG uses electro-anatomical modelling and proprietary algorithms. CineECG results can be influenced by the quality of the patient recorded ECG data (influenced by ECG electrodes positions on the torso, the orientation and rotation of the heart, the quality of the ECG signal recording device and other characteristics outside the control of ECG Excellence).

ECG Excellence