


# HP 03458-66509 (A9 reference board)

This is a clone of the reference board in the HP 3458A 8.5-digit multimeter.

See <https://github.com/pepaslabs/hp-03458-66509-clone>

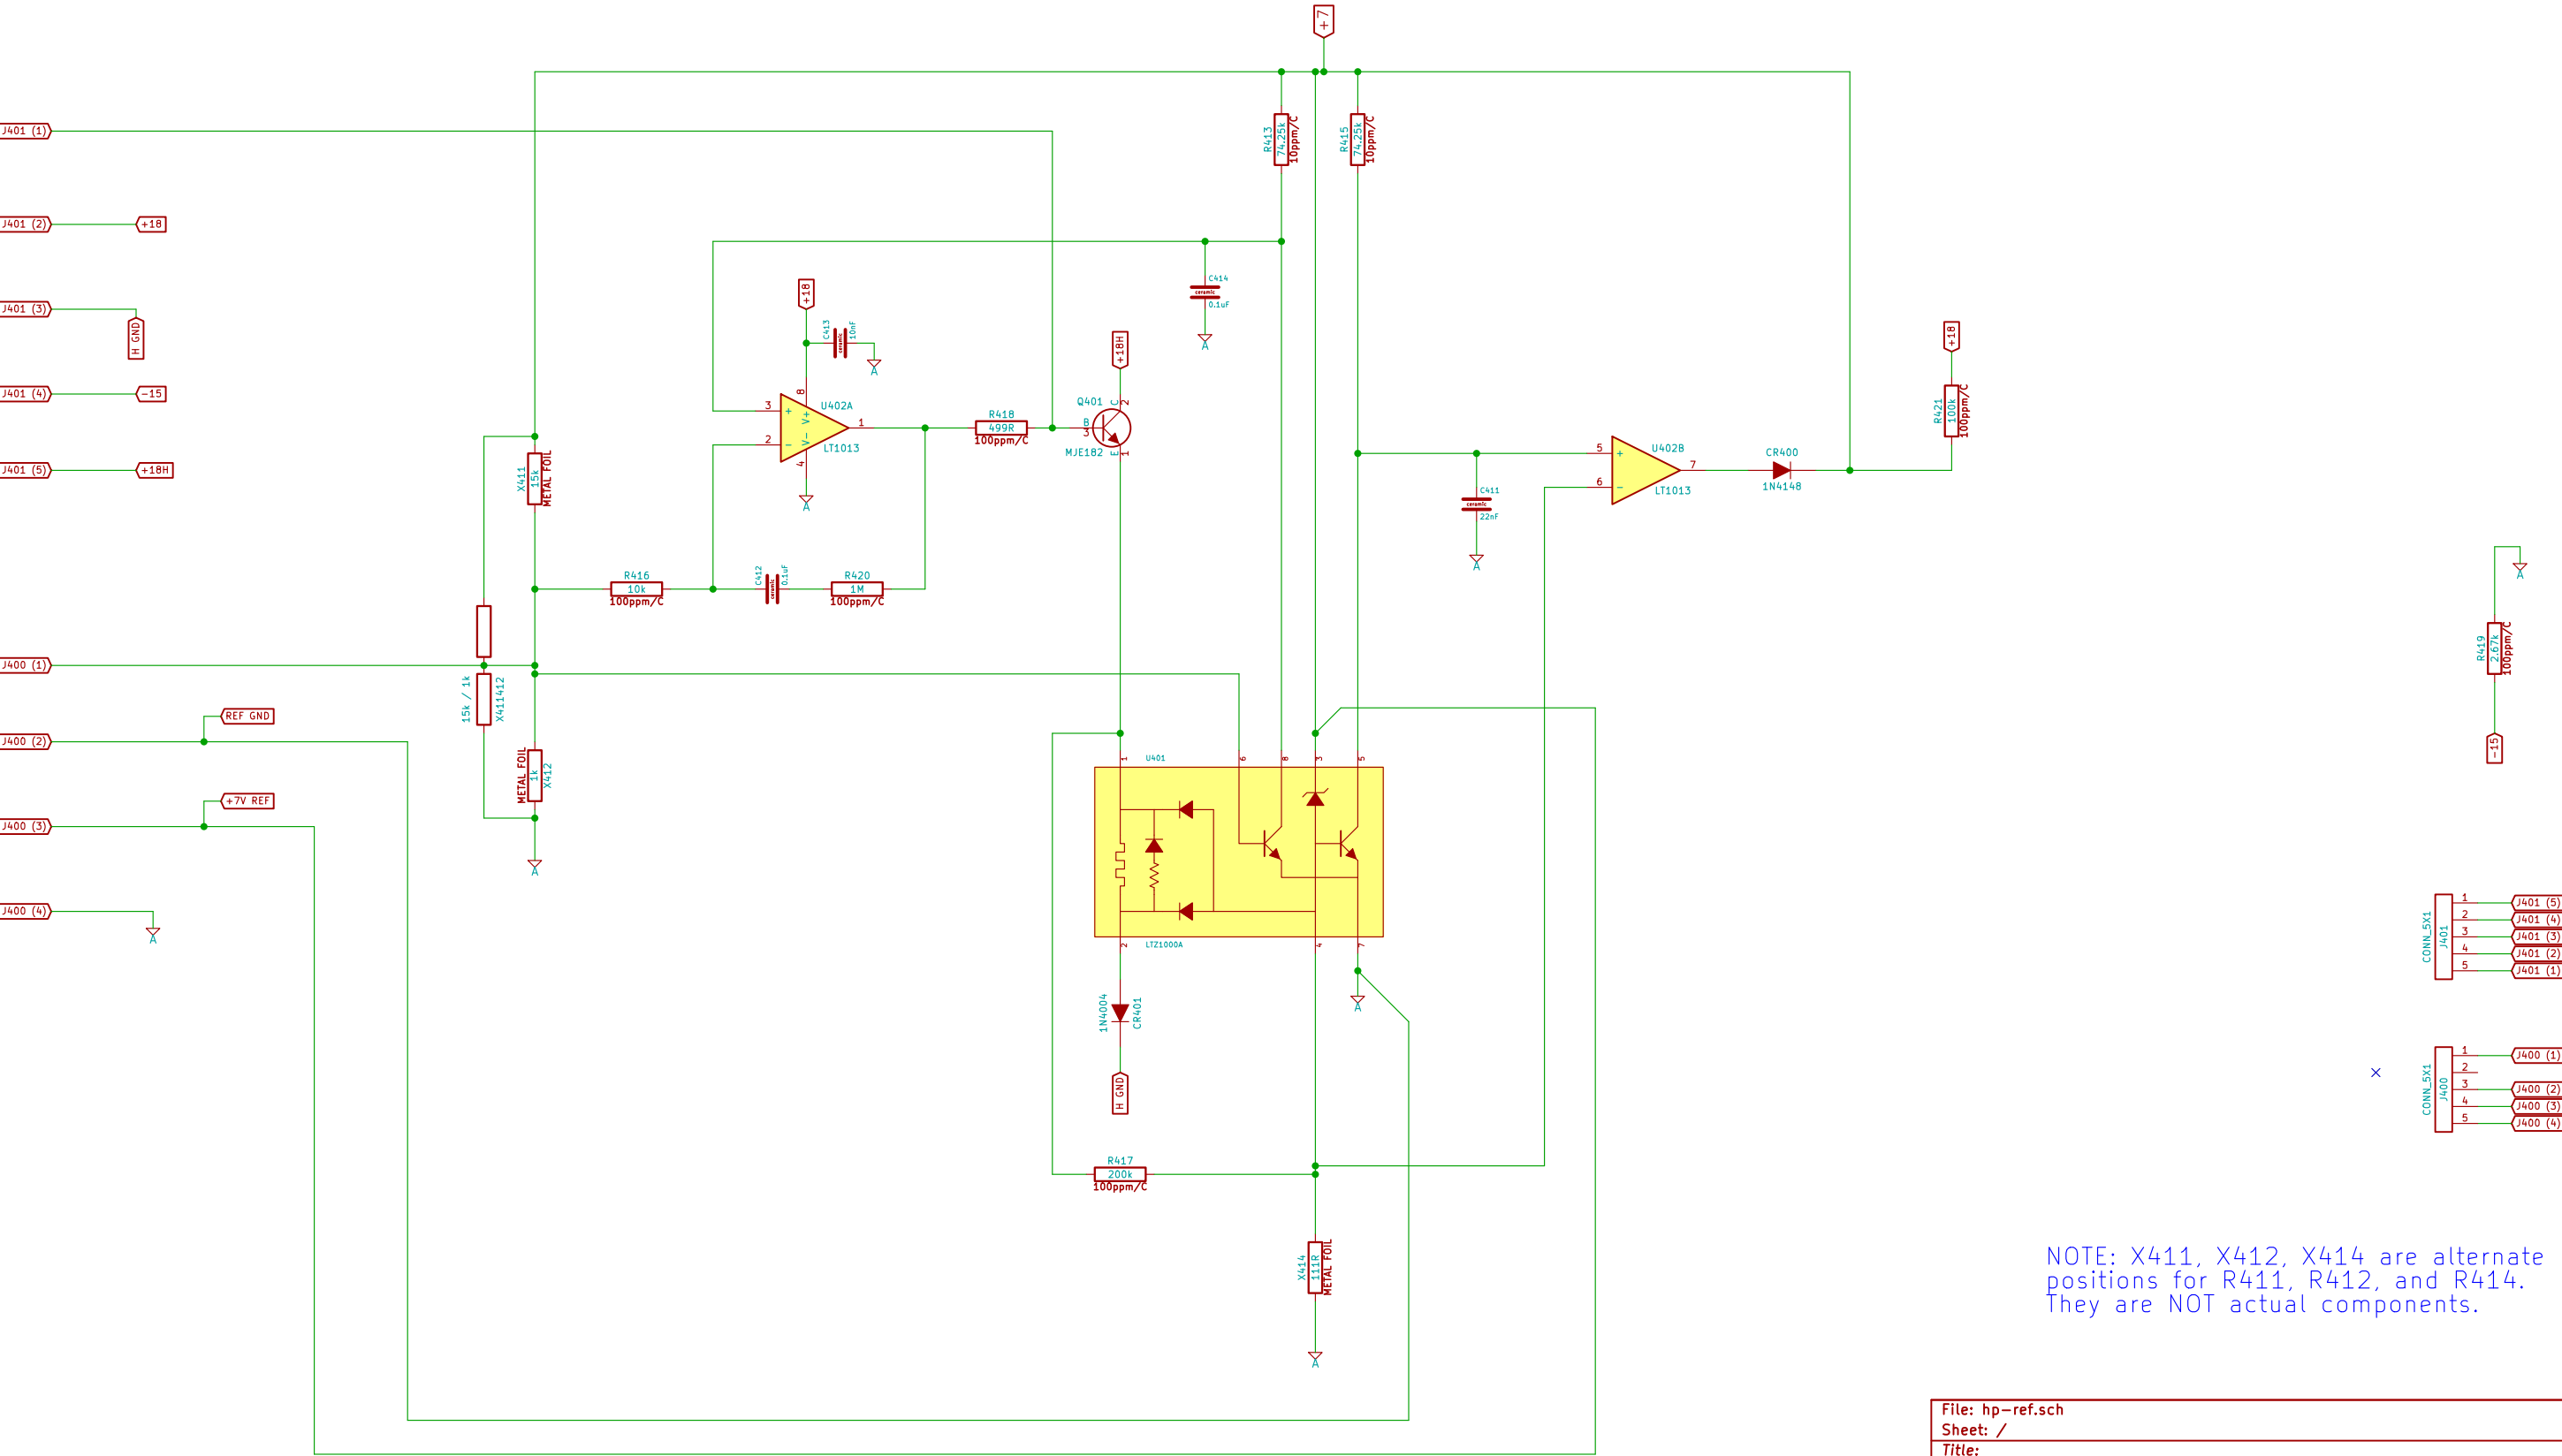

NOTE: X411, X412, X414 are alternate positions for R411, R412, and R414. They are NOT actual components.

|                  |                   |         |
|------------------|-------------------|---------|
| File: hp-ref.sch |                   |         |
| Sheet: /         |                   |         |
| Title:           |                   |         |
| Size: USLedger   | Date: 17 dec 2017 | Rev:    |
| KiCad E.D.A.     |                   | Id: 1/1 |