



**SURGICAL DIATHERMY**



## Features

- Monopolar cut: max 400W. Low, Pure, Blend & Endo Cut
- Monopolar coag: 120W. Desiccate, LCF Fulgurate, HCF Fulgurate & Spray
- Bipolar coag: 120W. Macro, Standard and Precise
- Bipolar Cut: 100W
- Vessel Seal : L-6, 150W, Auto-stop & regrasp Indicators
- Programmable power settings: 10 programs
- Tissue sensing technology
- Patient plate contact quality monitoring
- HF leakage monitoring

## Specifications

<b>Monopolar Cut</b>	In 300 $\Omega$
Blend	200 W
Pure	400 W
Low	300 W
Endo cut	200 W
<b>Monopolar Coagulation</b>	In 500 $\Omega$
Spray	120 W
Fulgurate LCF	120 W
Fulgurate HCF	120 W
Desiccate	120 W
<b>Bipolar Coagulation</b>	In 100 $\Omega$
Macro	120 W
Standard	070 W
Precise	120 W
<b>Bipolar Cut</b>	In 100 $\Omega$
Pure Cut	120 W
<b>Vessel Sealer</b>	In 100 $\Omega$
Levels	6 Levels
Power	Up to 150W



## Features

- Monopolar cut: max 400W. Low, Pure, Blend & Endo
- Monopolar coag: 120W. Desiccate, LCF Fulgurate, HCF Fulgurate & Spray
- Bipolar coag: 120W. Macro, Standard and Precise
- Bipolar Cut: 100W
- Programmable power settings: 10 programs
- Tissue sensing technology
- Patient plate contact quality monitoring
- HF leakage monitoring



## Specifications

<b>Monopolar Cut</b>	In 300 $\Omega$
Blend	200 W
Pure	400 W
Low	300 W
Endo cut	200 W
<b>Monopolar Coagulation</b>	In 500 $\Omega$
Spray	120 W
Fulgurate LCF	120 W
Fulgurate HCF	120 W
Desiccate	120 W
<b>Bipolar Coagulation</b>	In 100 $\Omega$
Macro	120 W
Standard	070 W
Precise	120 W
<b>Bipolar Cut</b>	In 100 $\Omega$
Pure Cut	120 W




#### Specifications

<b>Monopolar Cut</b>	In 300 $\Omega$
Blend	200 W
Pure	300 W
<b>Monopolar Coagulation</b>	In 500 $\Omega$
Spray	100 W
Fulgurate	100 W
Desiccate	120 W
<b>Bipolar Coagulation</b>	In 125 $\Omega$
Standard	070 W
<b>Bipolar Cut</b>	In 300 $\Omega$
Pure Cut	120 W

#### Features

- Monopolar cut: max 300W, 3 different blends.
- Monopolar coagulation: max 100W, Desiccate, Fulgurate & Spray modes
- Bipolar coagulation: 70W.
- Bipolar Cut: 120 W
- Programmable power settings: 10 Programs
- Patient plate contact quality monitoring

ACCESSORIES	Tailor 300	Tailor 400	Tailor Pro
Silicon Split Patient Plate	1	1	1
Cable for patient plate	1	1	1
Disposable handswitch, 3pin	1	1	1
Electrode set	1	1	1
Bipolar Forcep	1	1	1
Bipolar Cable	1	1	1
Monopolar foot switch	1	-	-
Bipolar Foot switch	1	-	-
Three pedal Foot switch	-	1	1
Vessel sealing laparoscopic instrument with cable	-	-	1
Biclamp With Cable	-	-	1
Power Cord	1	1	1

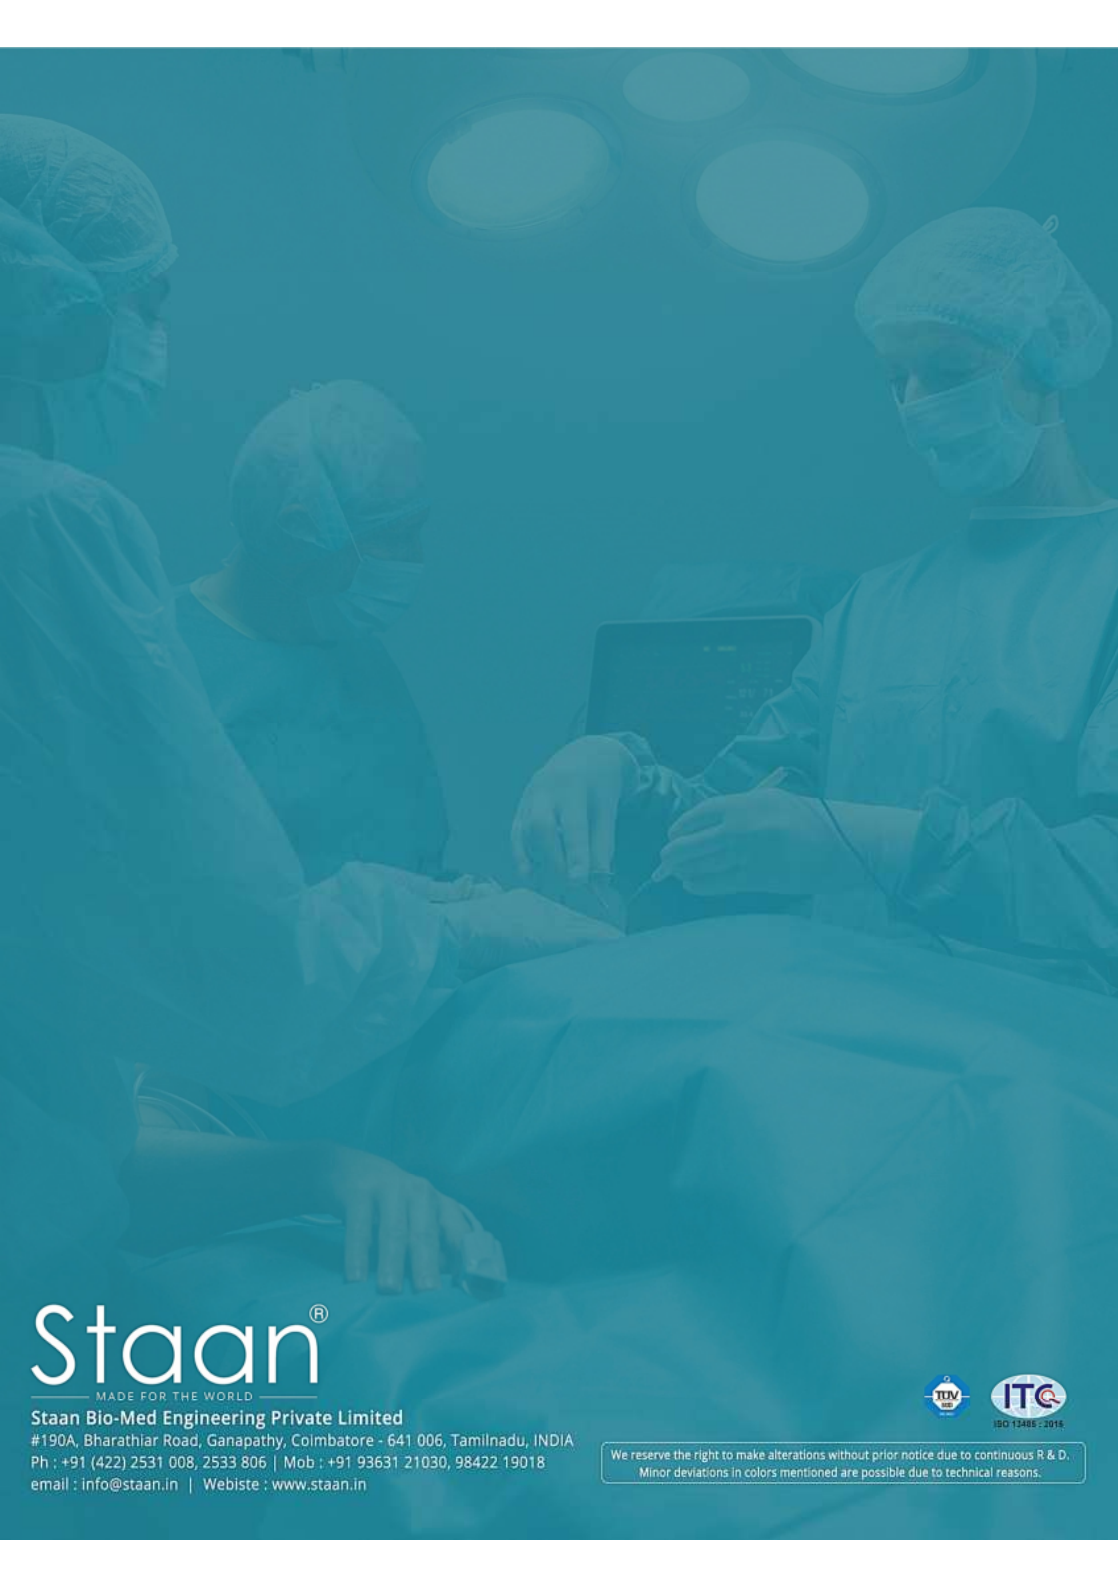

# Staan<sup>®</sup>

MADE FOR THE WORLD

**Staan Bio-Med Engineering Private Limited**

#190A, Bharathiar Road, Ganapathy, Coimbatore - 641 006, Tamilnadu, INDIA

Ph : +91 (422) 2531 008, 2533 806 | Mob : +91 93631 21030, 98422 19018

email : [info@staan.in](mailto:info@staan.in) | Website : [www.staan.in](http://www.staan.in)



ISO 13485 : 2016

We reserve the right to make alterations without prior notice due to continuous R & D.  
Minor deviations in colors mentioned are possible due to technical reasons.