



US 20250248831A1

(19) **United States**

(12) **Patent Application Publication**
Parsons et al.

(10) **Pub. No.: US 2025/0248831 A1**

(43) **Pub. Date: Aug. 7, 2025**

(54) **DURABLE STENT GRAFT WITH TAPERED STRUTS AND STABLE DELIVERY METHODS AND DEVICES**

A61F 2/89 (2013.01)

A61F 2/91 (2013.01)

A61F 2/95 (2013.01)

A61F 2/966 (2013.01)

(71) Applicant: **TriVascular, Inc.**, Santa Rosa, CA (US)

(52) **U.S. Cl.**

(72) Inventors: **Dennis Parsons**, Santa Rosa, CA (US);
Christopher L. Staudenmayer, Santa Rosa, CA (US); **James R. Watson**, Santa Rosa, CA (US)

CPC *A61F 2/90* (2013.01); *A61F 2/07*

(2013.01); *A61F 2/82* (2013.01); *A61F 2/848*

(2013.01); *A61F 2/91* (2013.01); *A61F*

2002/065 (2013.01); *A61F 2002/067*

(2013.01); *A61F 2002/072* (2013.01); *A61F*

2002/075 (2013.01); *A61F 2002/825*

(2013.01); *A61F 2/88* (2013.01); *A61F 2/89*

(2013.01); *A61F 2/95* (2013.01); *A61F*

2002/9665 (2013.01); *A61F 2210/0014*

(2013.01); *A61F 2220/0016* (2013.01); *A61F*

2220/005 (2013.01); *A61F 2220/0058*

(2013.01); *A61F 2220/0075* (2013.01); *A61F*

2230/0006 (2013.01); *A61F 2230/0008*

(2013.01); *A61F 2230/0013* (2013.01); *A61F*

2230/0019 (2013.01); *A61F 2230/0026*

(2013.01); *A61F 2230/0078* (2013.01); *A61F*

2250/0003 (2013.01); *A61F 2250/0036*

(2013.01); *Y10T 29/49863* (2015.01)

(21) Appl. No.: **19/172,387**

(22) Filed: **Apr. 7, 2025**

Related U.S. Application Data

(63) Continuation of application No. 17/465,751, filed on Sep. 2, 2021, now Pat. No. 12,268,621, which is a continuation of application No. 14/615,337, filed on Feb. 5, 2015, now Pat. No. 11,109,989, which is a continuation of application No. 13/799,207, filed on Mar. 13, 2013, now Pat. No. 8,992,595.

(60) Provisional application No. 61/620,362, filed on Apr. 4, 2012.

Publication Classification

(51) **Int. Cl.**

A61F 2/90 (2013.01)

A61F 2/06 (2013.01)

A61F 2/07 (2013.01)

A61F 2/82 (2013.01)


A61F 2/848 (2013.01)

A61F 2/88 (2006.01)

(57)

ABSTRACT

Some embodiments relate in part to endovascular prostheses and methods of deploying same. Embodiments may be directed more specifically to stent grafts and methods of making and deploying same within the body of a patient. Stent embodiments may include tapered struts for an even distribution of strain. Stent embodiments may also include portions which are enlarged in a circumferential direction which may be configured to stabilize the stent in a constrained state.

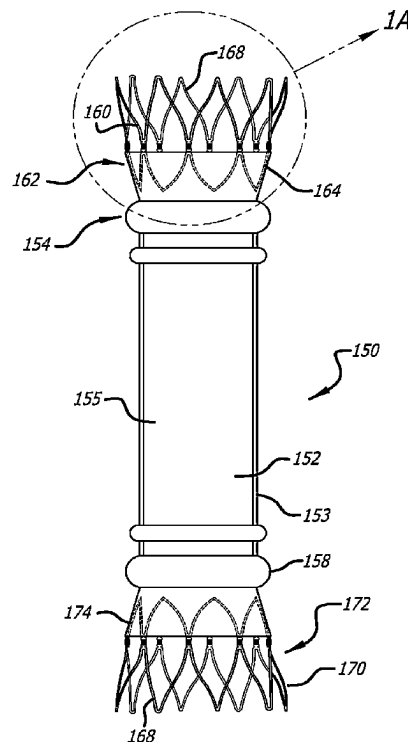

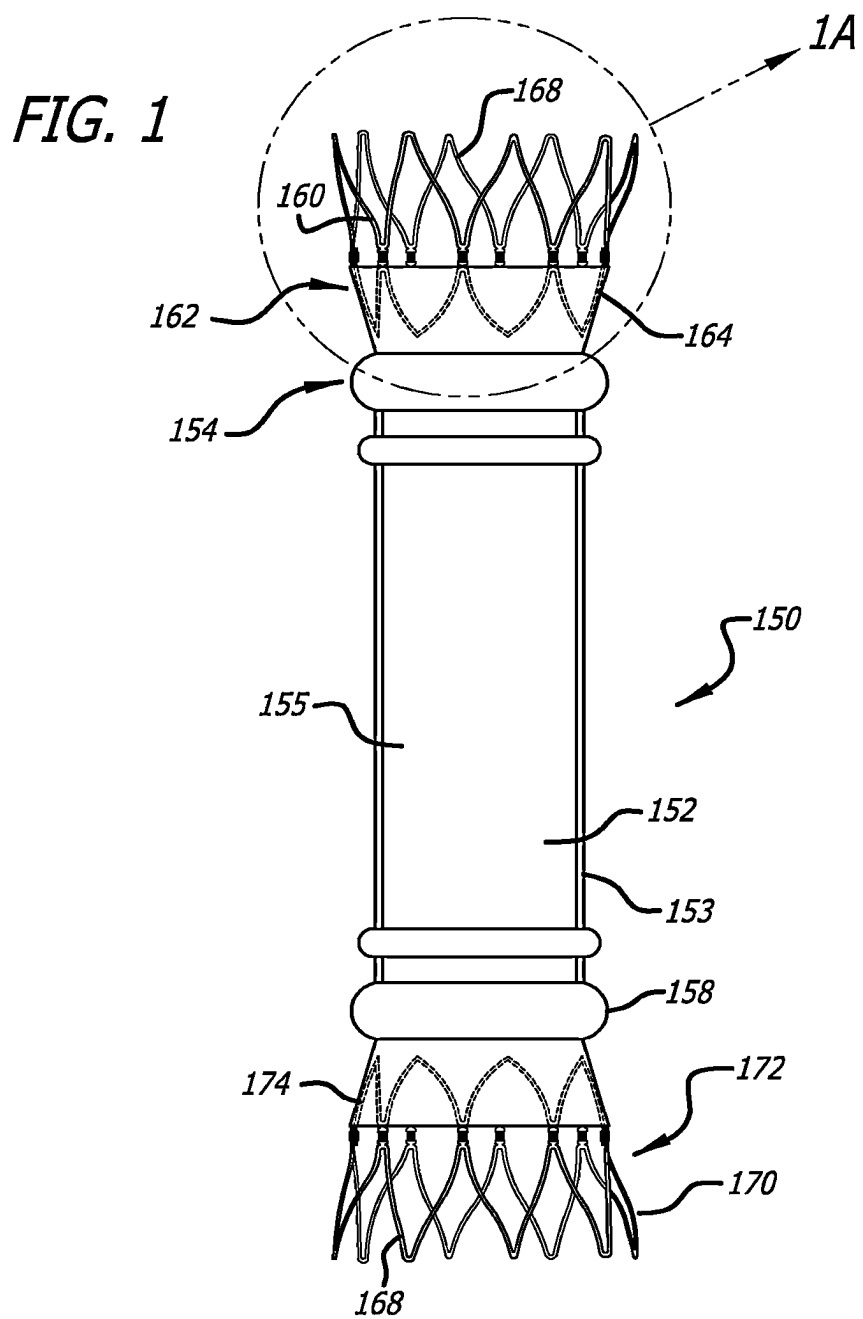
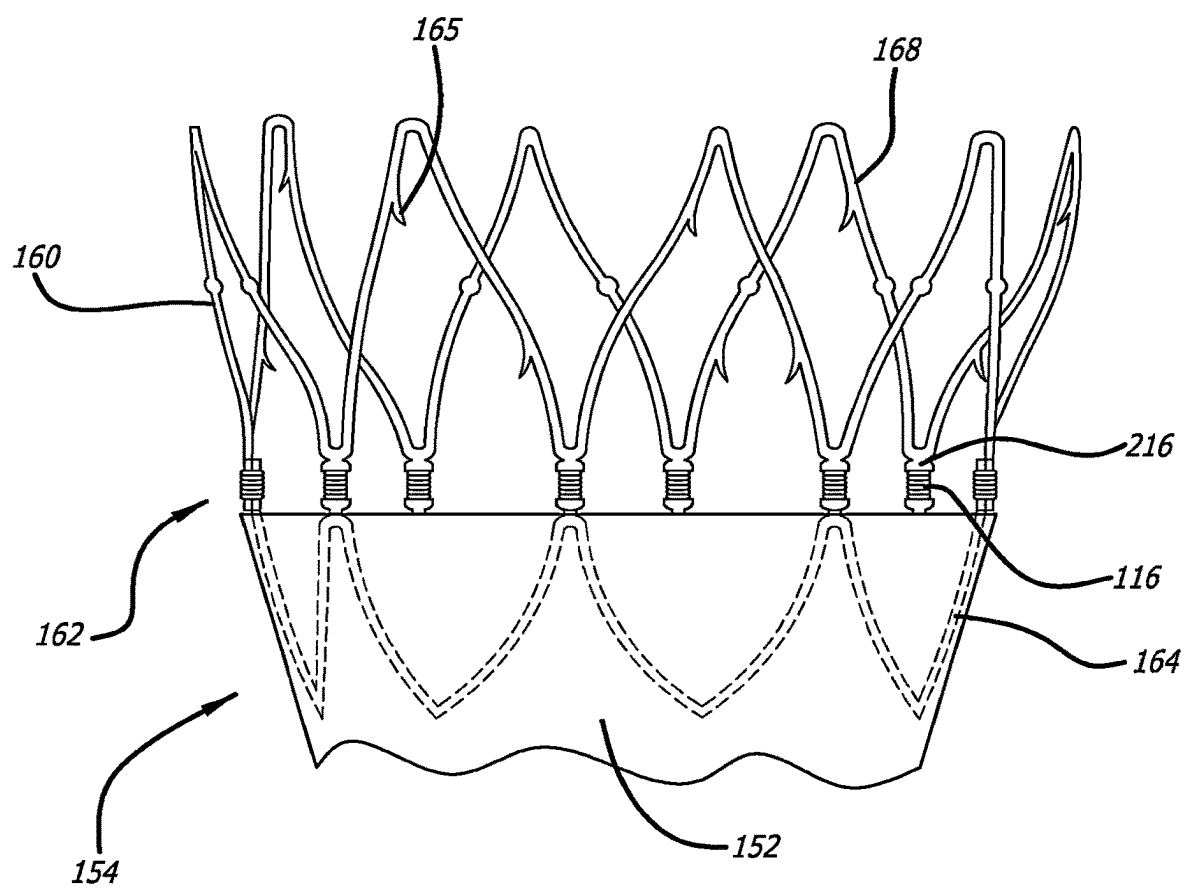
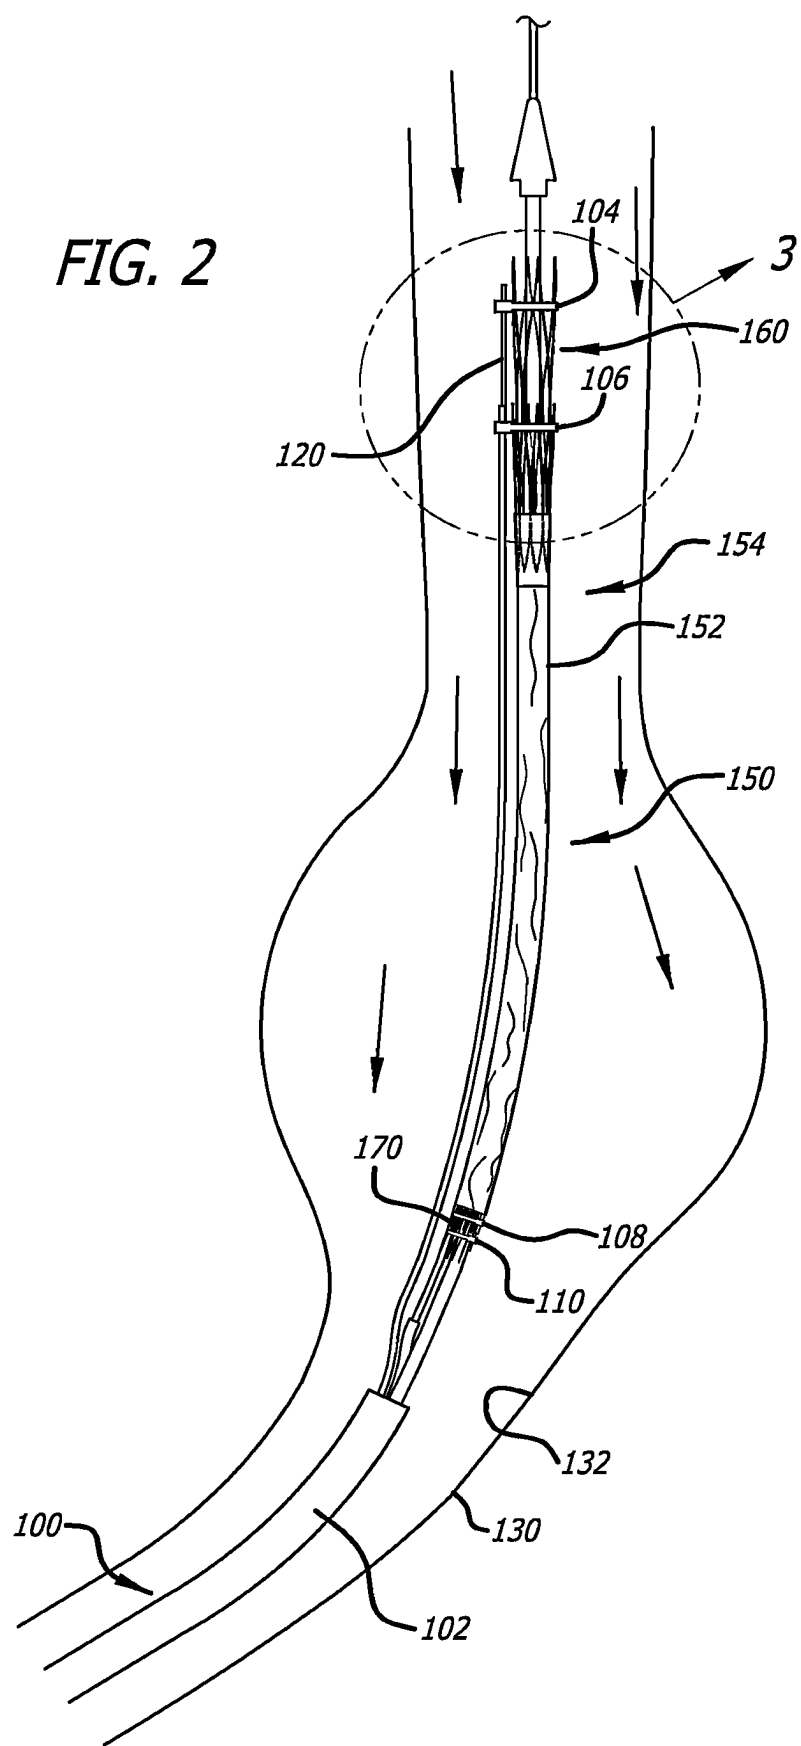


FIG. 1A





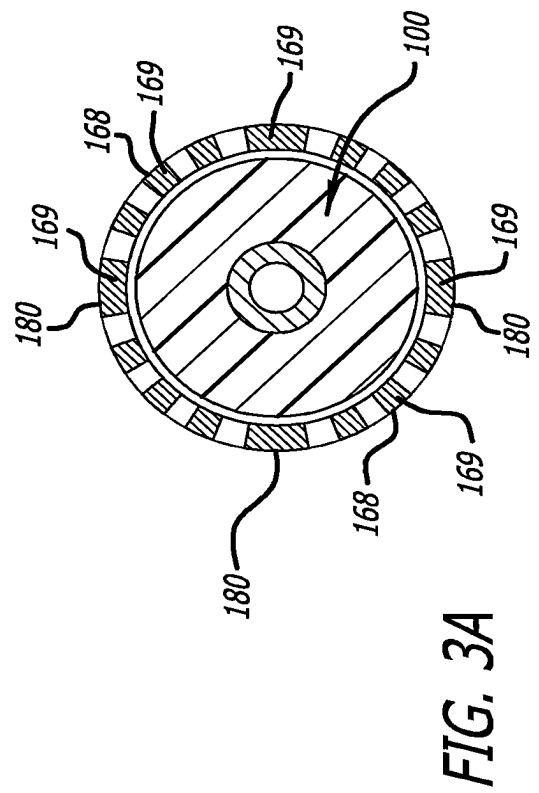
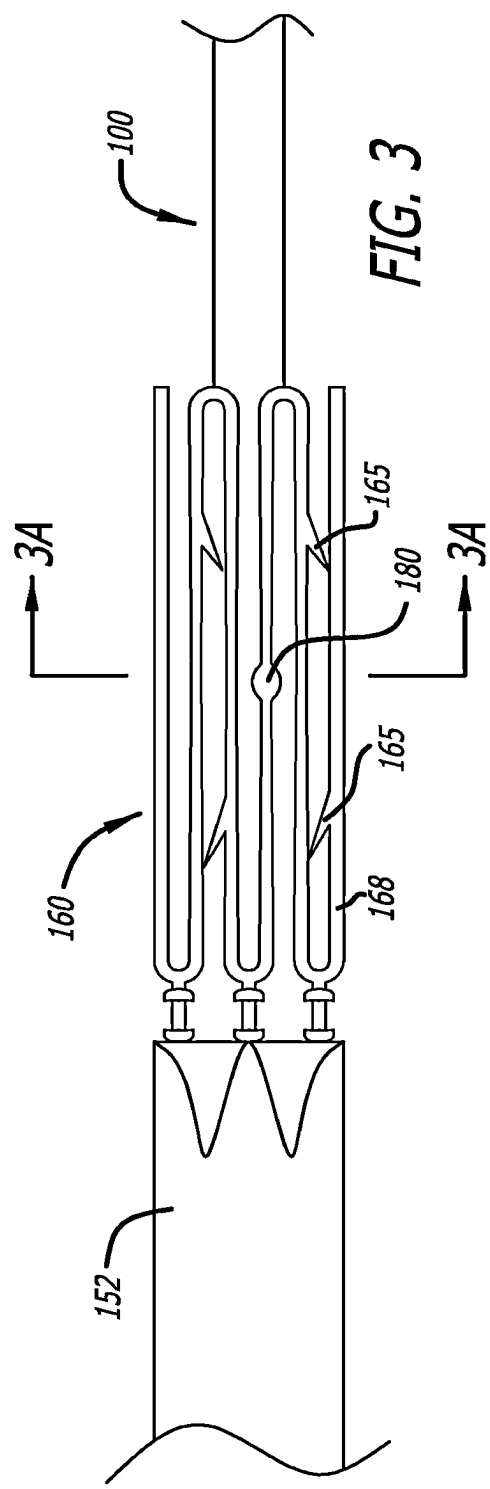
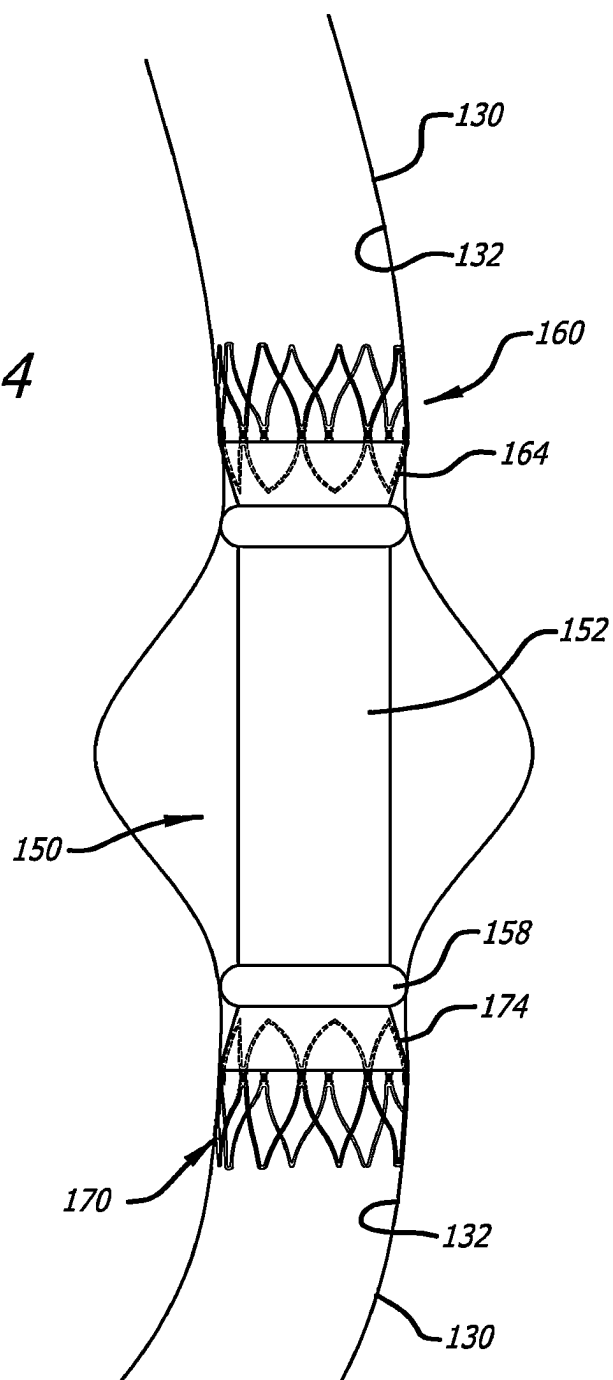


FIG. 4



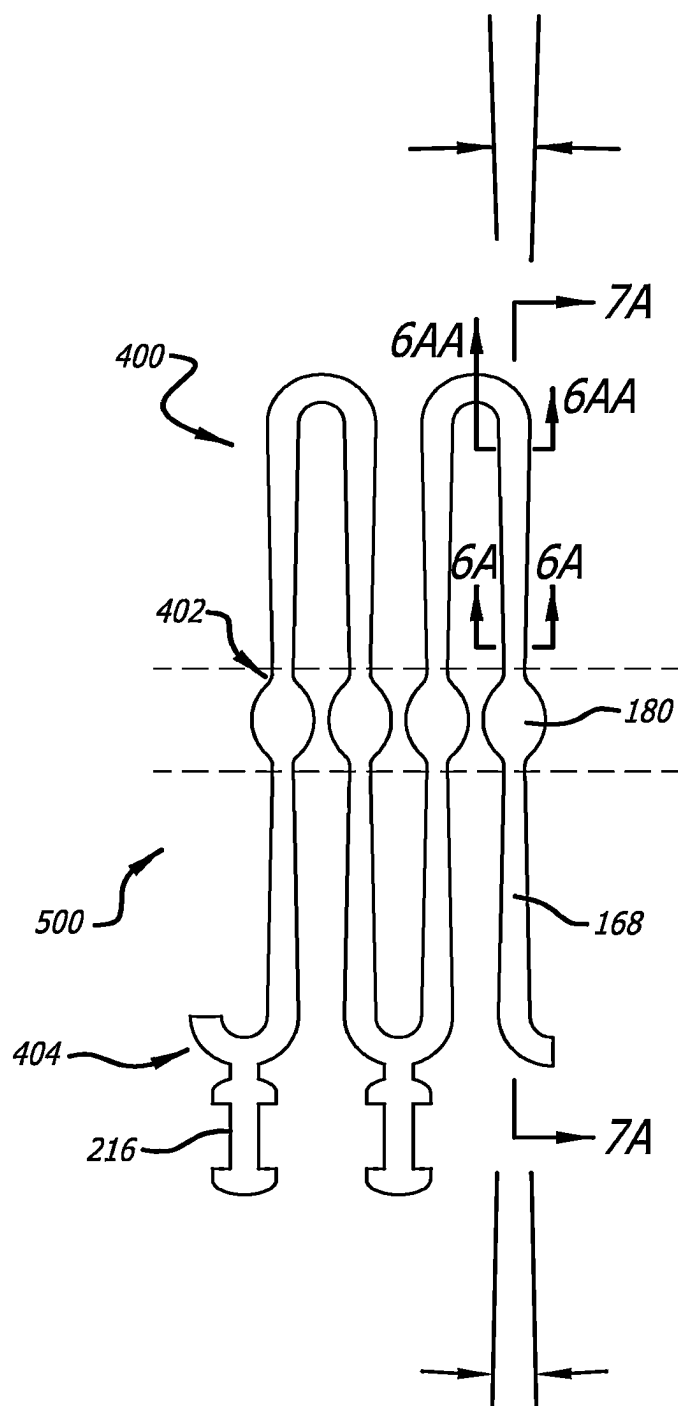


FIG. 5




FIG. 6A




FIG. 6AA




FIG. 6B

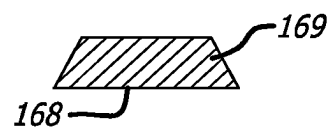


FIG. 6BB




FIG. 6C




FIG. 6CC




FIG. 6D

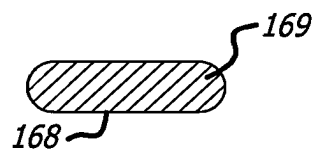


FIG. 6DD




FIG. 6E


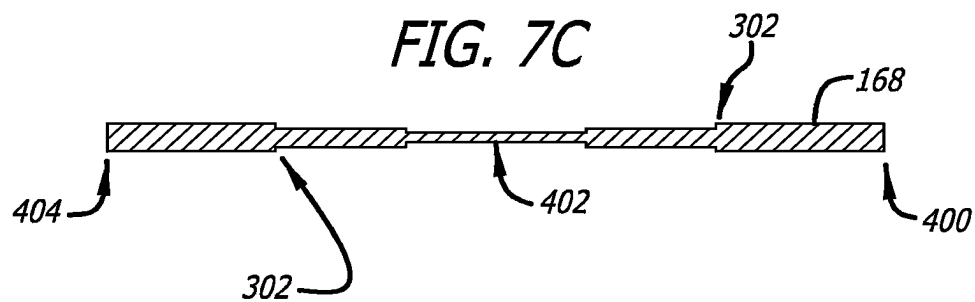
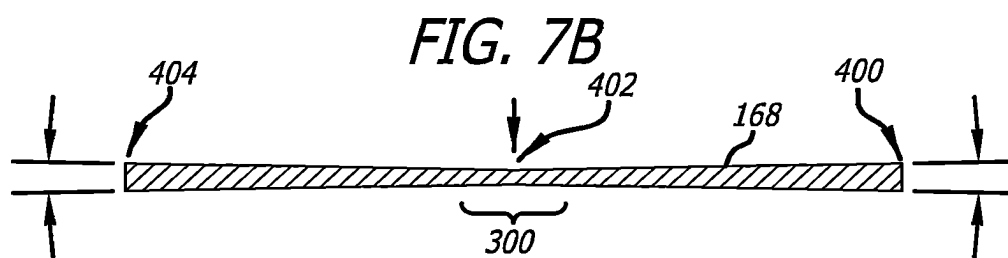
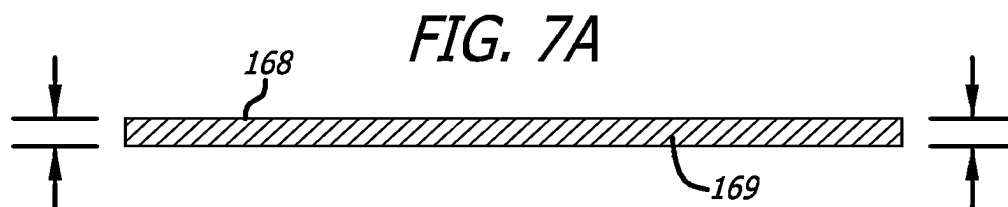
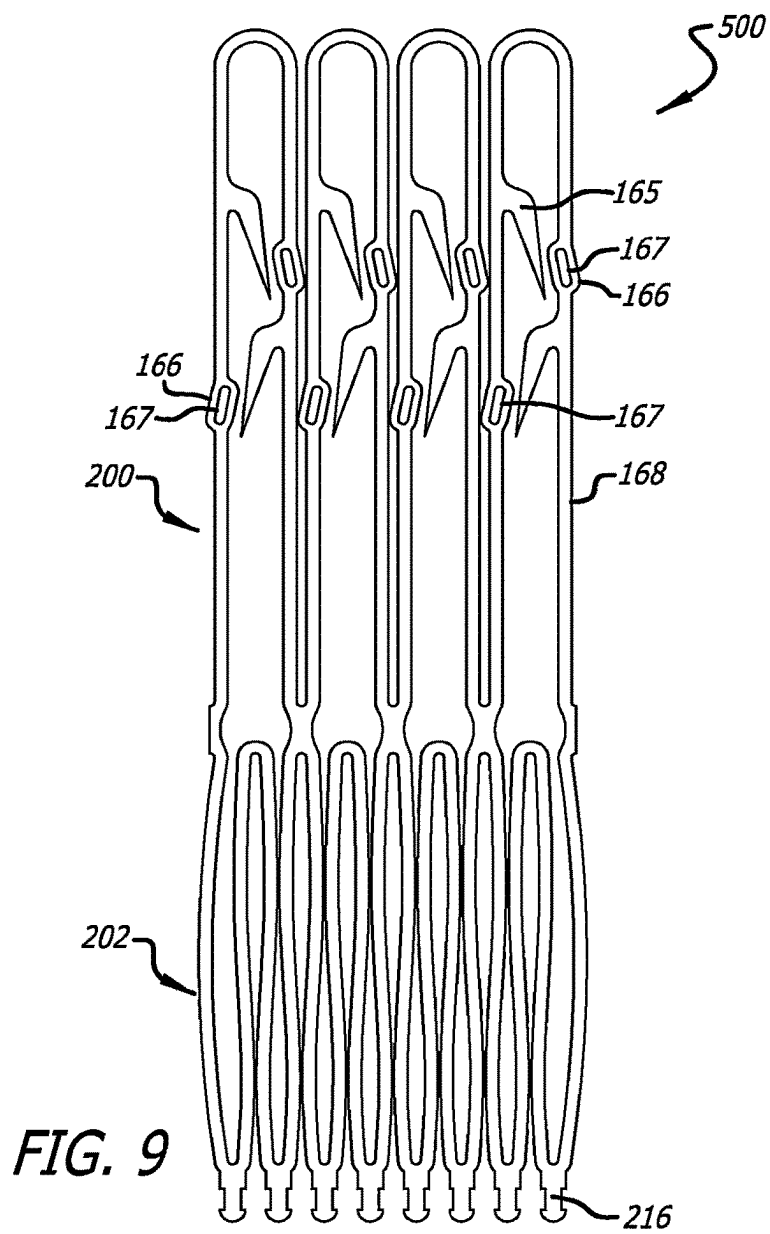
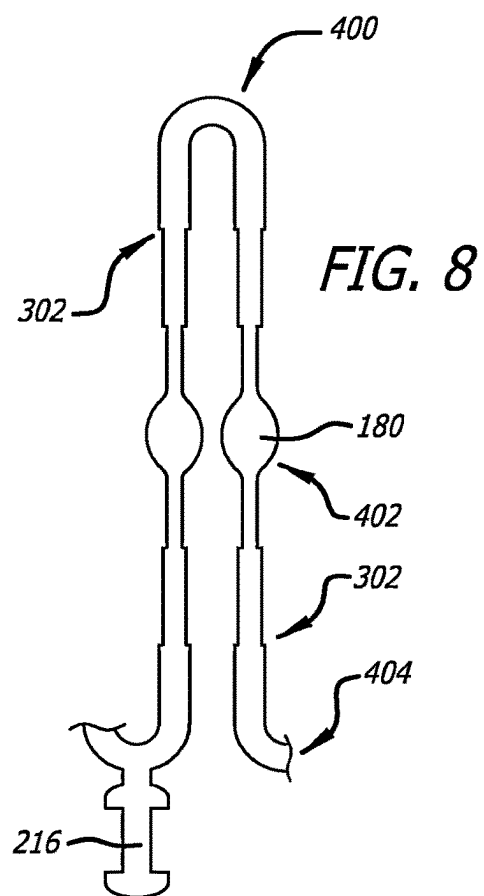


FIG. 6EE





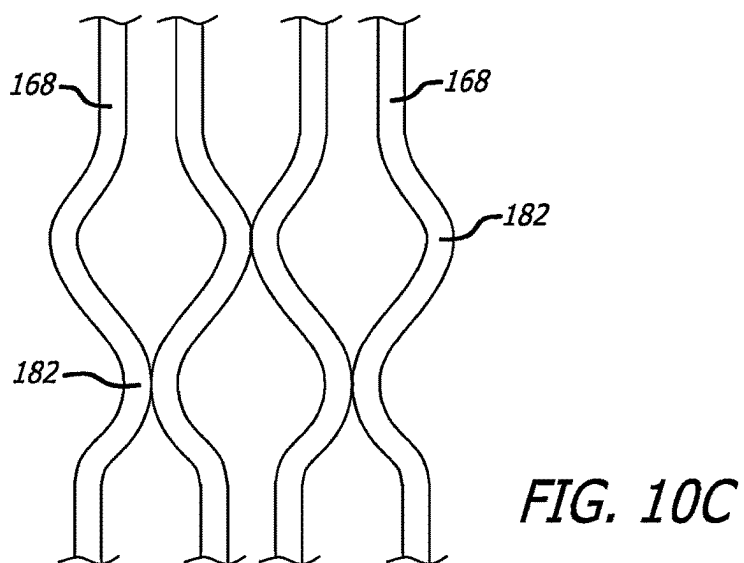
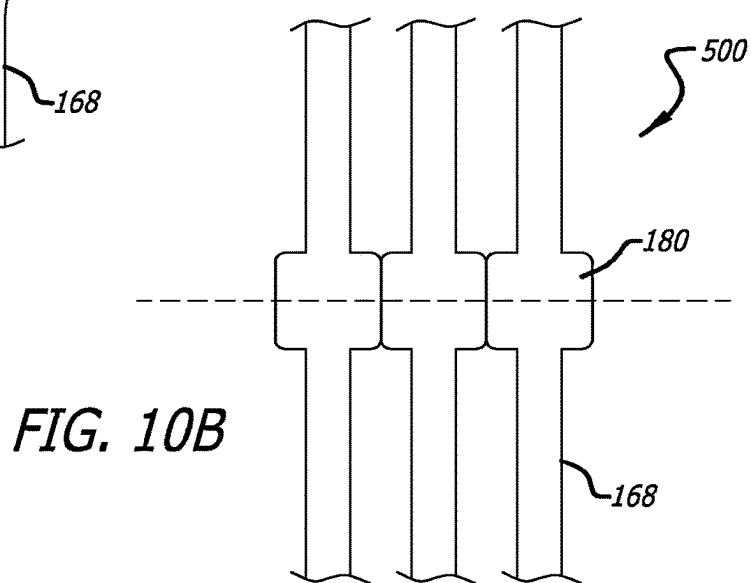
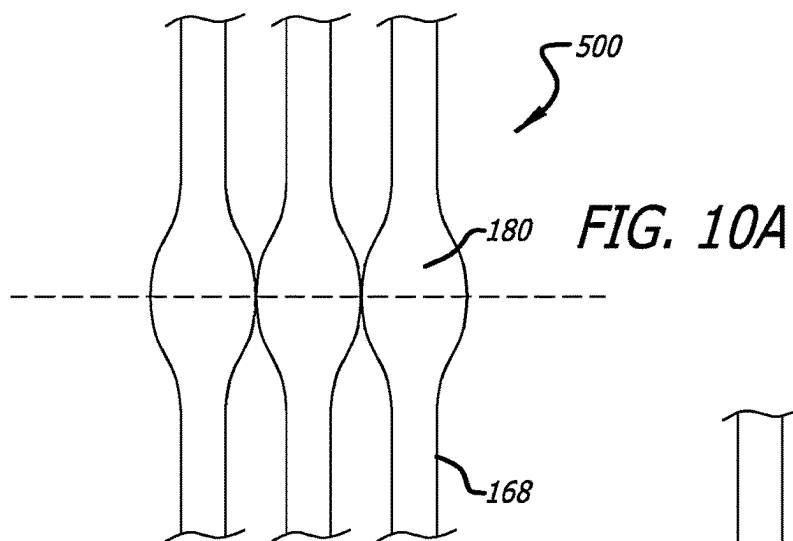




FIG. 13

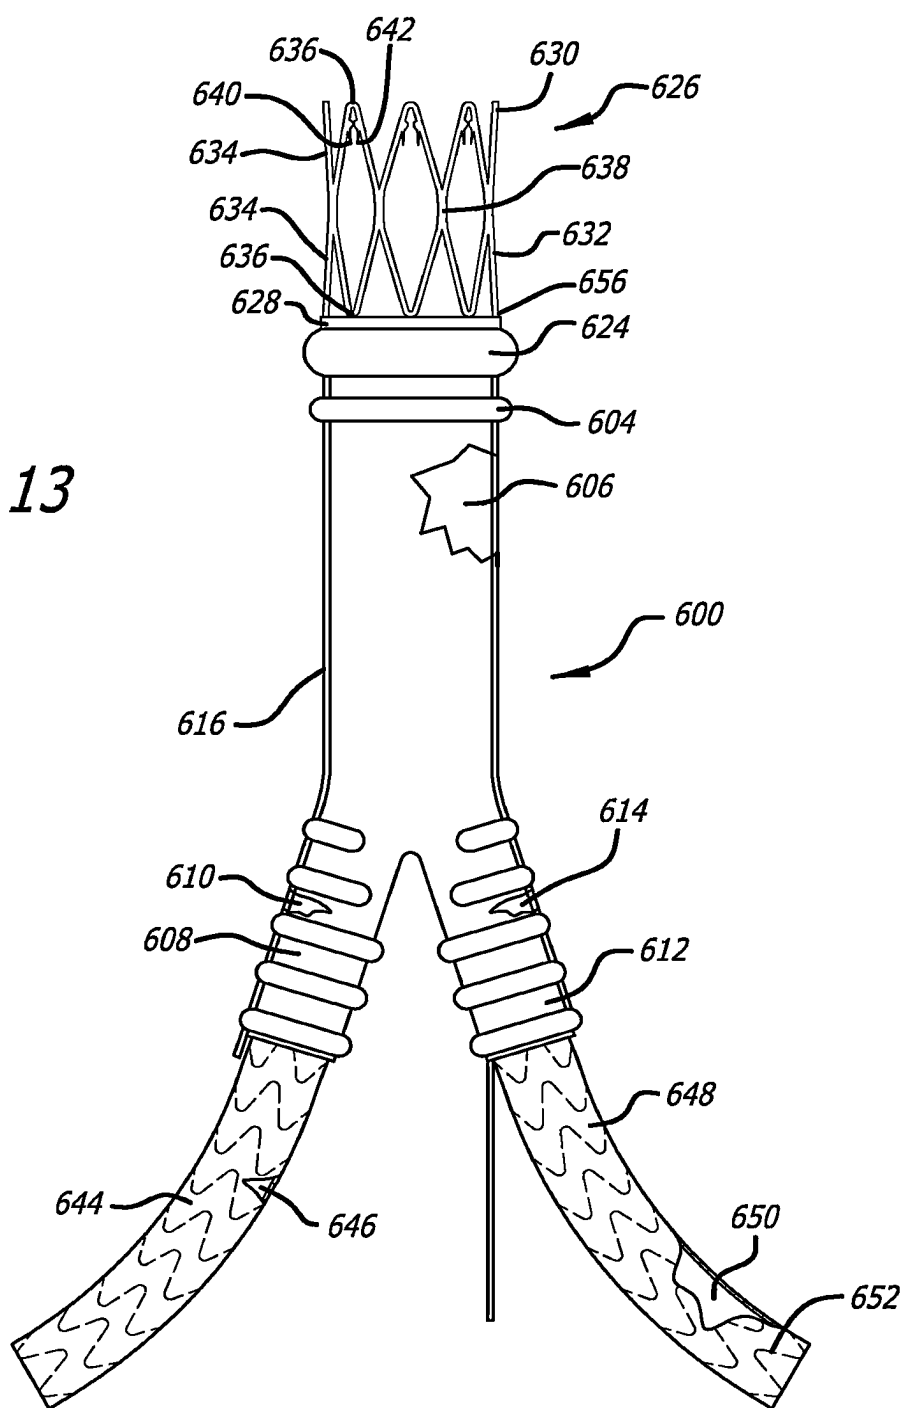
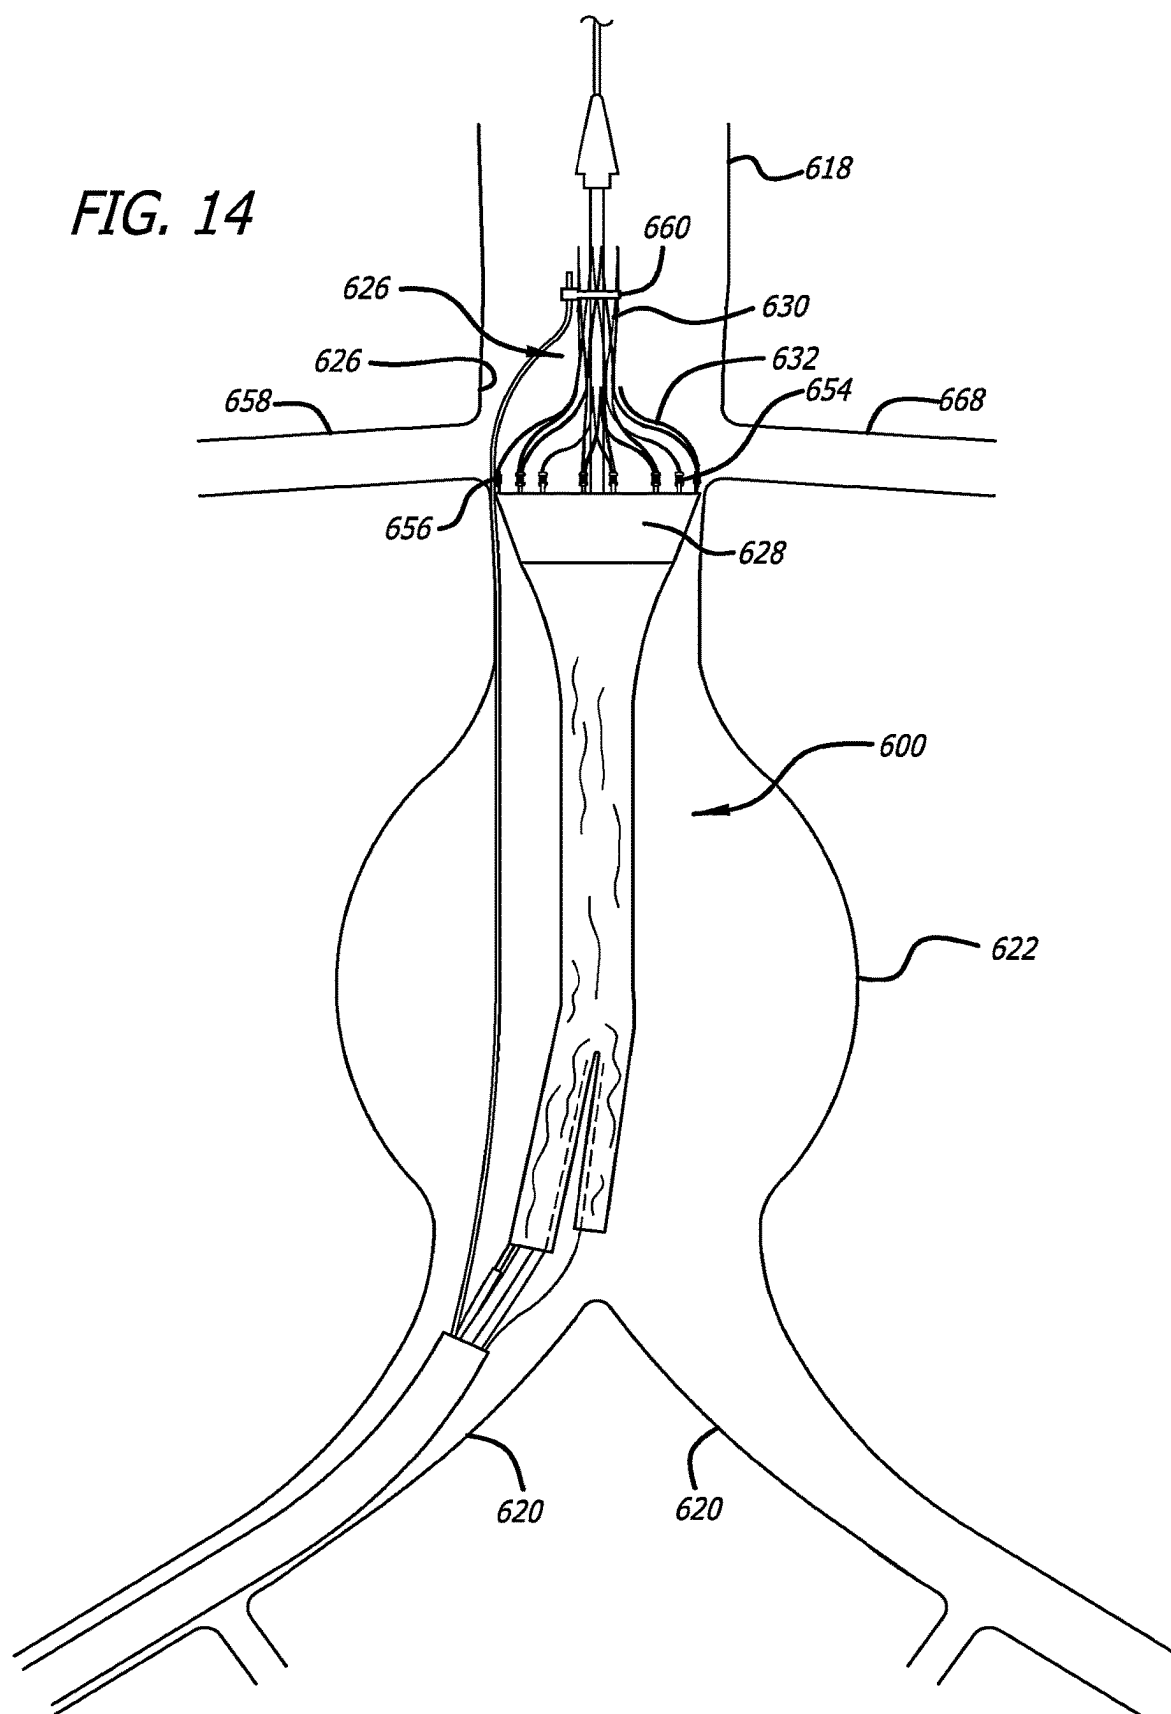
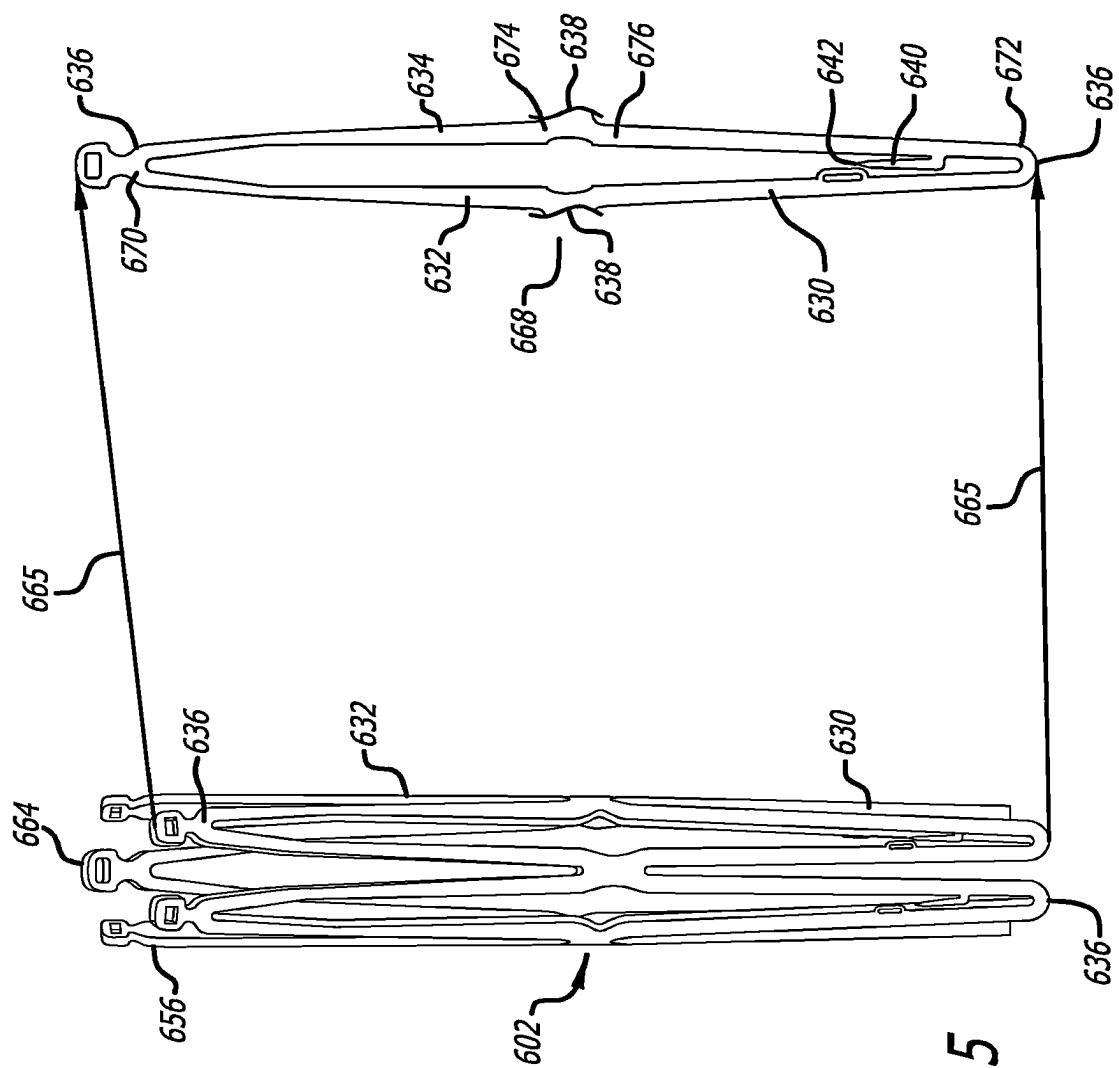


FIG. 14







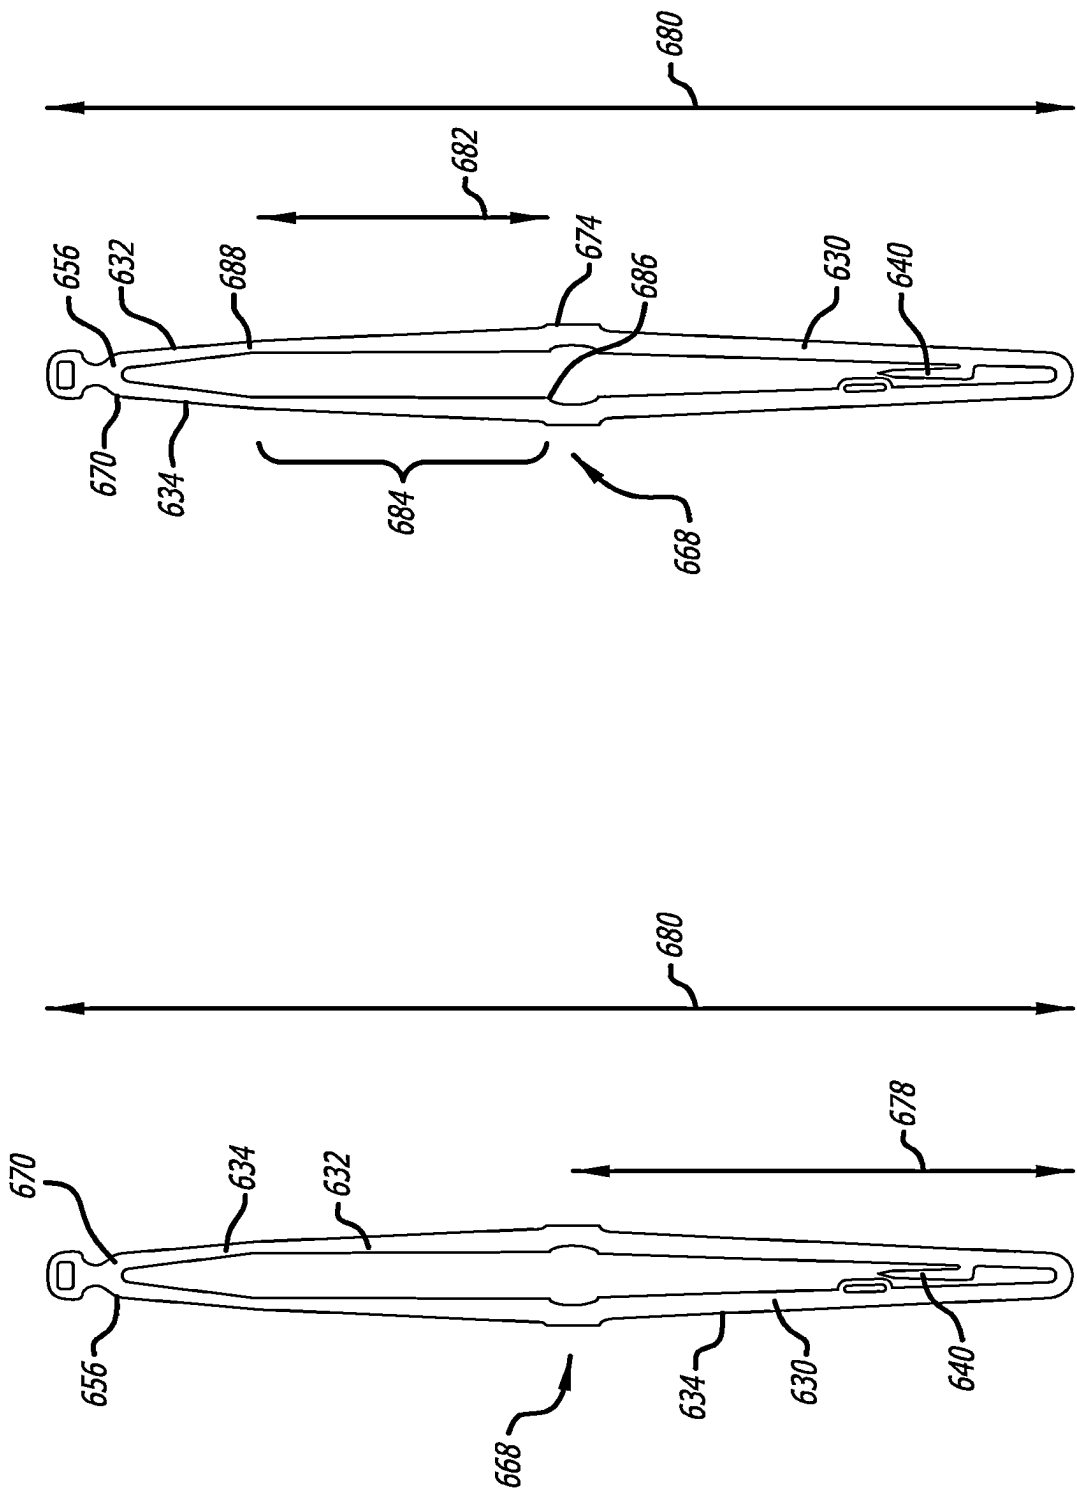


FIG. 17

FIG. 16

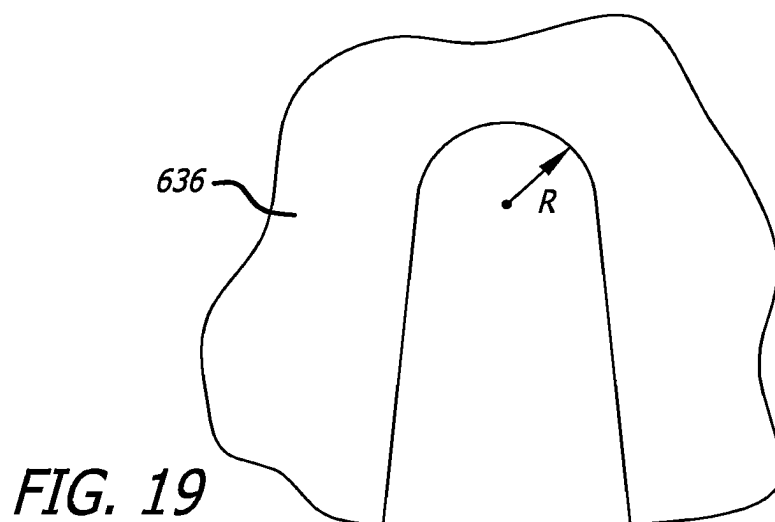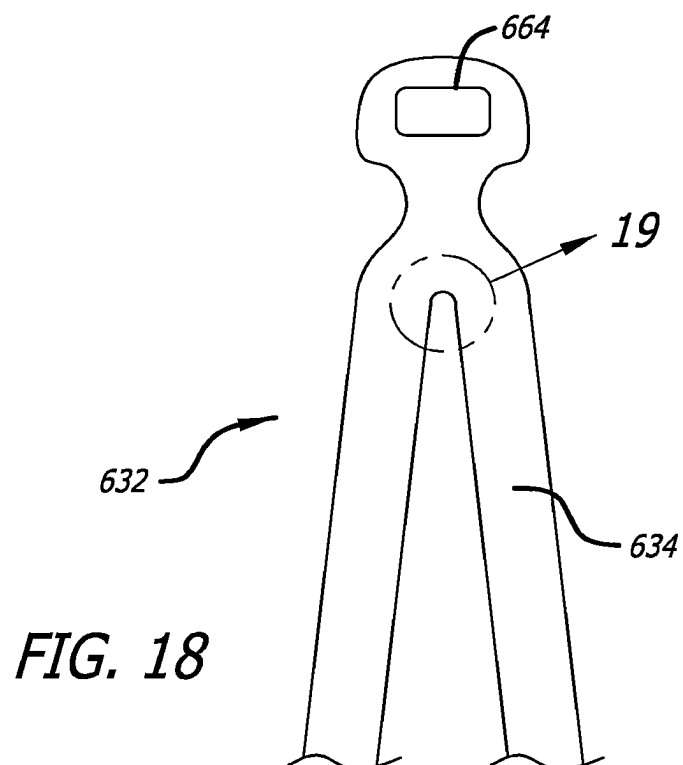

DURABLE STENT GRAFT WITH TAPERED STRUTS AND STABLE DELIVERY METHODS AND DEVICES

RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 17/465,751, filed Sep. 2, 2021, which is a continuation of U.S. patent application Ser. No. 14/615,337, filed Feb. 5, 2015, which is a continuation of U.S. patent application Ser. No. 13/799,207, filed Mar. 13, 2013, by D. Parsons et al., titled Durable Stent Graft with Tapered Struts and Stable Delivery Methods and Devices, which claims priority under 35 U.S.C. 119(e) from U.S. Provisional Patent Application No. 61/620,362, filed Apr. 4, 2012, by D. Parsons et al., titled Durable Stent Graft with Tapered Struts and Stable Delivery Methods and Devices, each of which is incorporated by reference herein in its entirety.

FIELD OF THE INVENTION

[0002] Some embodiments relate in part to endovascular prostheses and methods of deploying same. Embodiments may be directed more specifically to stent grafts and methods of making and deploying same within the body of a patient.

BACKGROUND

[0003] An aneurysm is a medical condition indicated generally by an expansion and weakening of the wall of an artery of a patient. Aneurysms can develop at various sites within a patient's body. Thoracic aortic aneurysms (TAAs) or abdominal aortic aneurysms (AAAs) are manifested by an expansion and weakening of the aorta which is a serious and life threatening condition for which intervention is generally indicated. Existing methods of treating aneurysms include invasive surgical procedures with graft replacement of the affected vessel or body lumen or reinforcement of the vessel with a graft.

[0004] Surgical procedures to treat aortic aneurysms can have relatively high morbidity and mortality rates due to the risk factors inherent to surgical repair of this disease as well as long hospital stays and painful recoveries. This is especially true for surgical repair of TAAs, which is generally regarded as involving higher risk and more difficulty when compared to surgical repair of AAAs. An example of a surgical procedure involving repair of a AAA is described in a book titled Surgical Treatment of Aortic Aneurysms by Denton A. Cooley, M.D., published in 1986 by W. B. Saunders Company.

[0005] Due to the inherent risks and complexities of surgical repair of aortic aneurysms, endovascular repair has become a widely-used alternative therapy, most notably in treating AAAs. Early work in this field is exemplified by Lawrence, Jr. et al. in "Percutaneous Endovascular Graft: Experimental Evaluation", Radiology (May 1987) and by Mirich et al. in "Percutaneously Placed Endovascular Grafts for Aortic Aneurysms: Feasibility Study," Radiology (March 1989). Commercially available endoprotheses for the endovascular treatment of AAAs include the AneuRx® stent graft manufactured by Medtronic, Inc. of Minneapolis, MN, the Zenith® stent graft system sold by Cook, Inc. of Bloomington, IN, the PowerLink® stent-graft system manufactured by Endologix, Inc. of Irvine, CA, and the Excluder® stent graft system manufactured by W.L. Gore & Associates,

Inc. of Newark, DE. A commercially available stent graft for the treatment of TAAs is the TAG™ system manufactured by W.L. Gore & Associates, Inc.

[0006] When deploying devices by catheter or other suitable instrument, it is advantageous to have a flexible and low profile stent graft and delivery system for passage through the various guiding catheters as well as the patient's sometimes tortuous anatomy. Many of the existing endovascular devices and methods for treatment of aneurysms, while representing significant advancement over previous devices and methods, use systems having relatively large transverse profiles, often up to 24 French. Also, such existing systems have greater than desired lateral stiffness, which can complicate the delivery process. In addition, the sizing of stent grafts may be important to achieve a favorable clinical result. In order to properly size a stent graft, the treating facility typically must maintain a large and expensive inventory of stent grafts in order to accommodate the varied sizes of patient vessels due to varied patient sizes and vessel morphologies. Alternatively, intervention may be delayed while awaiting custom size stent grafts to be manufactured and sent to the treating facility. As such, minimally invasive endovascular treatment of aneurysms is not available for many patients that would benefit from such a procedure and can be more difficult to carry out for those patients for whom the procedure is indicated.

[0007] What have been needed are stent graft systems and methods that are adaptable to a wide range of patient anatomies and that can be safely and reliably deployed using a flexible low profile system.

SUMMARY

[0008] Some embodiments are directed to a self-expanding cylindrical stent which has a constrained state and a relaxed expanded state. The stent may also include a longitudinal axis, a proximal end, a distal end, and a plurality of resilient struts configured to exert an outward radial force in the constrained state. At least one of the resilient struts may include a longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and configured to stabilize the at least one strut relative to the position of adjacent struts while the stent is in a constrained state. At least some of the enlarged longitudinal sections may be in axial alignment with each other. In some cases, the enlarged longitudinal sections of the struts may be enlarged in one transverse dimension of the struts. In some cases, the enlarged longitudinal sections may be enlarged along a circumferential direction about the longitudinal axis of the stent and the struts may have a substantially constant thickness in a radial direction relative to the longitudinal axis of the stent. The enlarged longitudinal section may have an enlarged transverse dimension that is about 1.5 times to about 3 times the nominal transverse dimension of the strut in a direction of the enlargement for some embodiments.

[0009] Certain embodiments are directed to an endovascular stent graft, having a main body portion including at least one tubular portion made from at least one layer of flexible material and a self-expanding cylindrical stent which has a constrained state and a relaxed expanded state. The stent may also include a longitudinal axis, a proximal end, a distal end, a plurality of resilient struts configured to exert an outward radial force in the constrained state. At least one of the resilient struts may include a longitudinal

section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and configured to stabilize the at least one strut relative to the position of adjacent struts while the stent is in a constrained state. All resilient struts may include a longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and configured to stabilize at least one strut relative to the position of adjacent struts while the stent is in a constrained state in some embodiments. In some cases, at least some of the enlarged longitudinal sections may be in axial alignment with each other. In some instances, the enlarged longitudinal sections of the struts may be enlarged in one transverse dimension of the struts. In some instances, the enlarged longitudinal sections may be enlarged along a circumferential direction about the longitudinal axis of the stent and the struts may have a substantially constant thickness in a radial direction relative to the longitudinal axis of the stent. The enlarged longitudinal section may have an enlarged transverse dimension that is about 1.5 times to about 3 times the nominal transverse dimension of the strut in a direction of the enlargement in some embodiments.

[0010] Some embodiments are directed to a method of loading a delivery catheter system with an endovascular stent graft. The endovascular stent graft may have a main body portion including at least one tubular portion made from at least one layer of flexible material, and a self-expanding cylindrical stent which has a constrained state and a relaxed expanded state. The self-expanding cylindrical stent may include a longitudinal axis, a proximal end, a distal end, a plurality of resilient struts configured to exert an outward radial force in the constrained state. At least one of the resilient struts may include a longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and configured to separate and stabilize the at least one strut relative to the position of adjacent struts while the stent is in a constrained state. In some cases, the self-expanding cylindrical stent of the stent graft may be constrained about a bushing of the delivery system such that the enlarged longitudinal section of the at least one resilient strut stabilizes the position of the at least one strut relative to the position of adjacent struts in the constrained state. In some instances, the stent may be releasably secured in the constrained stabilized state.

[0011] Some embodiments of an endovascular stent graft may include a main body portion having at least one tubular portion made from at least one layer of flexible material and a self-expanding anchor member. The self-expanding anchor member may include a constrained state, a relaxed expanded state, a proximal stent portion, and a distal stent portion. In some cases, the endovascular stent graft may be configured such that a proximal end of the distal stent portion is secured to a distal end of the proximal stent portion and a distal end of the distal stent portion is secured to a proximal end of the main body portion. The endovascular stent graft may also be configured such that the axial length of the self-expanding anchor member as a whole divided by the axial length of the proximal stent portion is a ratio of about 1.75 to about 2.0.

[0012] Some embodiments of a self-expanding anchor member include a constrained state, a relaxed expanded state, a proximal stent portion, and a distal stent portion. In some cases, the anchor member may be configured such that a proximal end of the distal stent portion is secured to a distal end of the proximal stent portion and the axial length of the

self-expanding anchor member as a whole divided by the axial length of the proximal stent portion is a ratio of about 1.75 to about 2.0.

[0013] Some embodiments of an endovascular stent graft may include a main body portion including at least one tubular portion made from at least one layer of flexible material and a self-expanding cylindrical stent which has a constrained state and a relaxed expanded state. The self-expanding cylindrical stent may include a longitudinal axis, a proximal end, a distal end, and a plurality of resilient struts configured to exert an outward radial force in the constrained state. At least one of the resilient struts may have a longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and be configured to stabilize the at least one strut relative to the position of adjacent struts while the stent is in a constrained state. For such an embodiment, all of the resilient struts of the stent may include a longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and be configured to stabilize the at least one strut relative to the position of adjacent struts while the stent is in a constrained state. In some cases at least some of the enlarged longitudinal sections may be in axial alignment with each other. In some instances, the enlarged longitudinal sections of the struts may be enlarged in one transverse dimension of the struts or the enlarged longitudinal sections may be enlarged along a circumferential direction about the longitudinal axis of the stent and the struts may have a substantially constant thickness in a radial direction relative to the longitudinal axis of the stent. For some embodiments, the enlarged longitudinal section may have an enlarged transverse dimension that is about 1.5 times to about 3 times the nominal transverse dimension of the strut in a direction of the enlargement. In some cases, the enlarged longitudinal section includes an undulating configuration of the nominal strut or an oval enlargement of the nominal strut. In some instances, each strut of the stent may include an enlarged longitudinal section with only one enlarged longitudinal section or an enlarged longitudinal section with a plurality of enlarged longitudinal sections. For some embodiments, the struts having enlarged longitudinal sections may be disposed in a substantially longitudinal orientation between the proximal end and distal end of the stent when the stent is in the constrained state. In some cases, the struts may be disposed in an undulating pattern. In some instances, the self-expanding cylindrical stent of the stent graft may include a superelastic alloy such as NiTi alloy.

[0014] Certain embodiments are described further in the following description, examples, claims and drawings.

BRIEF DESCRIPTION OF THE DRAWINGS

[0015] FIG. 1 illustrates an elevation view of an embodiment of an endoluminal prosthesis in the form of a stent graft for treatment of a patient's vessel.

[0016] FIG. 1A is an enlarged view of the encircled portion 1A of FIG. 1 including a proximal self-expanding stent member and proximal connector ring of the stent graft embodiment of FIG. 1.

[0017] FIG. 2 illustrates the stent graft embodiment of FIG. 1 in a constrained configuration disposed on a distal section of a delivery catheter within a lumen of a patient's vessel.

[0018] FIG. 3 shows an enlarged view of the encircled portion 3 of the stent graft of FIG. 2 including the proximal self-expanding stent member in a constrained configuration but without the constraining releasable belts for clarity of illustration.

[0019] FIG. 3A is a transverse cross sectional view of the proximal self-expanding stent member and delivery catheter system of FIG. 3 taken along lines 3A-3A of FIG. 3.

[0020] FIG. 4 illustrates the stent graft of FIG. 2 in a deployed unconstrained state.

[0021] FIG. 5 is a schematic view of an embodiment of a section of a stent that illustrates features of struts of the stent.

[0022] FIGS. 6A and 6AA illustrate paired transverse cross section views of a strut embodiment of FIG. 5 taken along the lines 6A-6A and 6AA-6AA of FIG. 5.

[0023] FIGS. 6B and 6BB illustrate paired transverse cross section views of another strut embodiment of FIG. 5.

[0024] FIGS. 6C and 6CC illustrate paired transverse cross section views of another strut embodiment of FIG. 5.

[0025] FIGS. 6D and 6DD illustrate paired transverse cross section views of another strut embodiment of FIG. 5.

[0026] FIGS. 6E and 6EE illustrate paired transverse cross section views of another strut embodiment of FIG. 5.

[0027] FIG. 7A illustrates a strut embodiment in longitudinal section taken along lines 7A-7A of the stent embodiment in FIG. 5.

[0028] FIG. 7B illustrates another strut embodiment in longitudinal section.

[0029] FIG. 7C illustrates another strut embodiment in longitudinal section.

[0030] FIG. 8 illustrates a portion of an embodiment of a stent including struts having a stepped taper configuration.

[0031] FIG. 9 illustrates a portion of an embodiment of a stent including struts having a continuous taper, barbs, and tuck pads with tuck slots.

[0032] FIG. 10A illustrates a portion of a cylindrical stent embodiment in a constrained configuration including struts having coaxial enlarged portion embodiments.

[0033] FIG. 10B illustrates a portion of a cylindrical stent embodiment in a constrained configuration including struts having coaxial enlarged portion embodiments.

[0034] FIG. 10C illustrates a portion of a cylindrical stent embodiment in a constrained configuration including struts having undulating deflected portions configured to physically separate adjacent struts in a circumferential direction.

[0035] FIG. 11 illustrates a portion of a cylindrical stent embodiment in a constrained configuration shown flattened including struts having coaxial enlarged portion embodiments and undulating deflected portions.

[0036] FIG. 12 is a transverse cross section view of the stent portion of FIG. 11 taken along lines 12-12 of FIG. 11.

[0037] FIG. 13 is an elevation view of a bifurcated stent graft embodiment.

[0038] FIG. 14 illustrates an embodiment of the stent graft of FIG. 13 partially deployed within a patient's aorta.

[0039] FIG. 15 is a perspective view of a proximal anchor member embodiment.

[0040] FIG. 16 is an elevation view of a cut away portion of the proximal anchor member embodiment of FIG. 15.

[0041] FIG. 17 is an elevation view of a cut away portion of the proximal anchor member embodiment of FIG. 16.

[0042] FIG. 18 shows a distal portion of the cut away portion of the proximal anchor member of FIG. 16.

[0043] FIG. 19 is an enlarged view of the encircled portion 19-19 in FIG. 18.

[0044] The drawings illustrate embodiments of the invention and are not limiting. For clarity and ease of illustration, the drawings are not made to scale and, in some instances, various aspects may be shown exaggerated or enlarged to facilitate an understanding of particular embodiments.

DETAILED DESCRIPTION

[0045] Embodiments of the invention are directed generally to methods and devices for treatment of fluid flow vessels with the body of a patient. Treatment of blood vessels may be specifically indicated for some embodiments, and, more specifically, treatment of aneurysms, such as abdominal aortic aneurysms. Devices for such treatment modalities may include stents, grafts and stent graft assemblies that include at least one stent secured to a graft member.

[0046] For some embodiments, the modular graft assembly may be bifurcated for treatment of an abdominal aortic aneurysm. Such a graft assembly embodiment may include a bifurcated main body member, an ipsilateral graft extension and contralateral graft extension. The main body may have a wall portion that binds a main fluid flow lumen disposed therein. An ipsilateral leg of the main body may have an ipsilateral port and an ipsilateral fluid flow lumen that is in fluid communication with the main fluid flow lumen and the ipsilateral port. A contralateral leg of the main body may have a contralateral port and a contralateral fluid flow lumen that is in fluid communication with the main fluid flow lumen and the contralateral port. The main body, ipsilateral leg, and contralateral leg may form a bifurcated "Y" shaped configuration.

[0047] For some bifurcated embodiments, the main fluid flow lumen of the main body generally may have a larger transverse dimension and area than a transverse dimension and area of either of the fluid flow lumens of the ipsilateral leg or contralateral leg. A proximal anchor member may be disposed at a proximal end of the main body. The proximal anchor member may include a proximal self-expanding stent that is formed from an elongate element having a generally serpentine shape with four crowns or apices at either end. Each proximal apex or crown of the proximal stent may be coupled to alternating distal crowns or apices of an eight crown distal self-expanding stent. The distal self-expanding stent may be formed from an elongate element having a generally serpentine shape. A distal end of the distal stent may be mechanically coupled to a connector ring which may be embedded in graft material of the proximal end of the main body, or directly coupled to perforations in the proximal edge region of the main body. Embodiments of the connector ring may be generally circular in shape having regular undulations about the circumference that may be substantially sinusoidal in shape. The proximal stent may include outwardly extending barbs, that may be integrally formed with the struts of the stent for some embodiments, having sharp tissue penetrating tips that are configured to penetrate into tissue of an inside surface of a lumen within which the proximal stent is deployed in an expanded state. Although the proximal anchor member may include self-expanding stents, similar stents may be used that are configured to be inelastically expanded with outward radial pressure as might be generated by the expansion of an

expandable balloon from within either or both stents. The connector ring coupled to the proximal stent may also be inelastically expandable.

[0048] With regard to graft embodiments discussed herein, such as graft assembly, and components thereof, as well as graft extensions and, the term “proximal” refers to a location towards a patient’s heart and the term “distal” refers to a location away from the patient’s heart. With regard to delivery system catheters and components thereof discussed herein, the term “distal” refers to a location that is disposed away from an operator who is using the catheter and the term “proximal” refers to a location towards the operator.

[0049] FIGS. 1-4 illustrate an embodiment of a stent graft assembly **150** which may include a main graft member or main body portion **152** which is not bifurcated. The main body **152** may be tubular in shape and have a wall portion **153** that bounds a main fluid flow lumen **155** disposed therein. The main body **152** may include a proximal end **154**, a distal end **156** and an inflatable portion **158**. The main body **152** of the stent graft assembly **150** may include at least one flexible layer of material such as PTFE, polymer meshes, composites of same or the like. A proximal anchor member or stent may be disposed at the proximal end **154** of the main body **152**. The proximal anchor member embodiment shown in FIG. 1 includes a single proximal self-expanding stent member **160** disposed about a proximal end **154** of the main body **152**. In some embodiments, the proximal self-expanding stent member **160** may be formed from an elongate element having a generally serpentine shape with eight crowns or apices at either end. A distal end **162** of the proximal self-expanding stent member **160** may be mechanically coupled to a proximal connector ring **164** which may be embedded in graft material generally about the proximal end **154** of the main body **152**, or directly coupled to perforations in the proximal end **154** region of the main body **152**.

[0050] A distal self-expanding stent member **170** may be disposed at the distal end **156** of the main body **152** and may be configured to engage an interior luminal surface **132** within the patient’s vasculature **130**. The distal self-expanding stent member **170** shown in FIG. 1 includes a single self-expanding stent member disposed along the distal end **156** of the main body **152** of the stent graft assembly **152**. The distal self-expanding stent member **170** may be formed from a resilient elongate element having a generally serpentine shape with eight crowns or apices at either end. A proximal end **172** of the distal self-expanding stent member **170** may be mechanically coupled to a distal connector ring **174** which may be embedded in graft material generally about the distal end **156** of the main body **152**, or directly coupled to perforations in the distal end **156** region of the main body **152**.

[0051] Embodiments of either the proximal connector ring **164** or distal connector ring **174** may be generally circular or cylindrical in shape with regular undulations about the circumference that may be substantially sinusoidal or zig-zag in shape. Some embodiments of either the proximal or distal self-expanding stent members **160**, **170** may include outwardly extending barbs **165** (see FIG. 1A). Such barbs **165** may be integrally formed with the struts **168** of either the proximal self-expanding stent member **160** or distal self-expanding member **170**. Furthermore, the barbs **165** may have sharp tissue penetrating tips that may be configured to penetrate into tissue of an inside surface of a lumen

within which either the proximal self-expanding stent member **160** or distal self-expanding member **170** may be deployed into an expanded state.

[0052] Although the proximal and distal self-expanding stent members **160** and **170** of the stent graft **150** has generally been described as including self-expanding stents, the proximal and distal self-expanding stent members **160** and **170** may also include similar stents that are configured to be inelastically expanded with outward radial pressure as might be generated by the expansion of an expandable balloon from within either the proximal self-expanding stent member **160** or distal self-expanding stent member **170**. Additionally, at least one of the proximal self-expanding stent member **160** and distal self-expanding stent member **170** may be made from or include a superelastic alloy, such as NiTi alloy.

[0053] The stent graft **150** may further include an optional inflation conduit (not shown) which may serve as a fill manifold for inflation of the inflatable portion **158** of the stent graft **150**. The inflation conduit may include a distal end with an inflation port in fluid communication with an exterior portion of the main body **152** and extending from the distal end **156** into an interior volume of the inflatable portion **158** of the stent graft **150**.

[0054] Some embodiments of the stent graft **150** may include radiopaque markers **116** that may be used to facilitate alignment of the stent graft **150**. A radiopaque marker **116** configuration and imaging system may be used for alignment during positioning of the stent graft **150** in a patient. FIG. 1A illustrates an enlarged view of a portion of the stent graft **150** with portions of the stent graft **150** not shown for clarity of illustration. The stent graft **150** embodiment shown in FIG. 1A illustrates the proximal end **154** of the main body **152**, the proximal self-expanding stent member **160**, and a plurality of radiopaque markers **116** disposed about a circumference of a distal end **162** of the proximal self-expanding stent member **160**. Furthermore, the plurality of radiopaque markers **116** may include helically wound wire members which may be disposed about connector members **216**, as shown in FIG. 1A. In general, the connector members **216** may be configured to mechanically couple the proximal self-expanding stent member **160** to the proximal connector ring **164** disposed within the proximal end **154** of the main body **152** of the stent graft **150**. Some embodiments of the stent graft **150** may additionally or alternatively include a plurality of radiopaque markers **116** circumferentially disposed about a tubular portion of the endovascular stent graft **150**. For example, the radiopaque markers **116** may lie in a plane that is substantially orthogonal or parallel to a longitudinal axis **186** of the tubular main body **152** of the stent graft **150**. Additionally, the distal self-expanding member **170** may include one or more radiopaque markers **116**.

[0055] Furthermore, any number of features may be incorporated into the stent graft **150** which may enable detection of all or part of the stent graft **150** under fluoroscopy or other suitable forms of imaging. For example, in general, the radiopaque markers **116**, or other detection features, may be used to facilitate orthogonal orientation of the imaging axis or view. Once a substantially orthogonal view angle is achieved, an accurate axial position of the partially deployed stent graft **150** relative to the patient’s vasculature may be achieved, avoiding parallax, ensuring precise placement of the stent graft **150** relative to significant branch vessels or

other anatomic reference points. Parallax in some circumstances may cause error in axial placement of the stent graft 150 relative to the intended target site. Accurate positioning may be achieved with axial movement and adjustment of the stent graft 150 by manual manipulation of a proximal portion of the delivery catheter 100.

[0056] As shown in FIG. 2, the stent graft 150 may be positioned such that the proximal end 154 of the main body 152 of the stent graft 150 is aligned distal of the ostium of the renal arteries. Once the delivery catheter 100 system has been positioned at the treatment site an outer sheath 102 of the delivery catheter 100 may be proximally retracted. Though the outer sheath 102 may have been proximally retracted, thus exposing the stent graft 150, the stent graft 150 may remain in a partially constrained state with the proximal self-expanding stent member 160 restrained by a pair of proximal releasable belts 104 and 106 releasably disposed about the proximal self-expanding stent member 160. The distal self-expanding stent member 170 may be constrained by another set of distal releasable belts 108 and 110 which may be releasably disposed about the distal self-expanding stent member 170.

[0057] Each of the releasable belts 104, 106, 108 and 110 may be configured to be independently released by retraction of one or more respective release wires 120. Release wires 120 may be disposed within an end loop or loops of the releasable belts 104, 106, 108 and 110 with the one or more release wires 120 holding the loops in fixed relation to each other. For this arrangement, retraction of one or more release wires 120 from the end loops releases the loops to allow them to move relative to each other which in turn removes the constraint of the belt members 104, 106, 108 and 110 about the respective proximal and distal self-expanding stent members 160 and 170. After at least partial deployment of the proximal stent member 160, finalizing the axial position of the stent graft 150 relative to the anatomy of the patient's vasculature 130 and treatment site may then be made. The axial positioning may be accomplished in some embodiments with the use of one or more radiopaque marker devices 116, as described above. Once the partially radially constrained stent graft 150 is axially aligned, the proximal self-expanding stent member 160 may then be fully deployed in order to engage and become secured to the luminal wall or interior luminal surface 132 of the patient's vasculature 130, as shown by way of example in FIG. 4. Once the proximal anchor member 160 is fully deployed, the inflatable portion 158 of the stent graft 150, including the network of inflatable channels, may be inflated with a fill material. For some embodiments, the network of inflatable channels may be filled from a desired site within the inflatable portion 158. More specifically, the inflatable portion 158 may be inflated with fill material from a proximal end 154 of the main body 152.

[0058] The proximal self-expanding stent member 160 may be disposed at and secured to a proximal end 154 of the main body 152. For example, the proximal self-expanding stent member 160 may have a first self-expanding stent member 200 secured to a second self-expanding stent member 202. Both the first and second self-expanding stent members 200 and 202 may have a somewhat tubular shape and may be secured together by one or more struts 168. Some embodiments of the struts 168 may have one or more cross sectional areas 169 that vary along the length of the strut 168. Such a configuration may be useful in avoiding

points of concentrated stress in, for example, the proximal self-expanding stent member 160 or struts 168. The proximal self-expanding stent member 160 may include at least one barb 165 and/or enlarged portion 180 on each strut 168, every other strut 168 or combinations thereof. One proximal self-expanding stent member 160 embodiment may have a repeated strut 168 pattern having a more proximally placed barb 165 on one strut 168, an adjacent neighbor strut 168 with a more distally placed barb 165, and a following adjacent strut 168 with a centrally placed enlarged portion 180, as shown in FIG. 3. Another enlarged portion embodiment 180 may have enlarged portions 180 on every strut 168, as shown in FIG. 5. Additionally, a proximal self-expanding stent member 160 embodiment may have a first self-expanding stent member 200 secured to a second self-expanding stent member 202 where the first self-expanding stent member 200 (or more proximal stent) may have alternating more distally placed barbs 165 along the struts 168 with more proximally placed barbs 165 along the struts 168, as shown in FIG. 9. Another proximal self-expanding stent member 160 embodiment may include one or more struts 168 having enlarged portions 180 generally centrally placed along the length of the struts 168, followed by alternating more distally placed barbs 165 with more proximally placed barbs 165 along the struts 168, as shown in FIG. 11.

[0059] For some embodiments, the first self-expanding member 200 of the proximal self-expanding stent member 160 may further include a plurality of barbs 165 having sharp tissue engaging tips that are configured to extend radially outward and distally in a deployed expanded state. This configuration may be useful in order to engage tissue of an inner luminal surface 132 of a patient's vasculature 130 and mechanically anchor the stent graft 150 to the vasculature 130, in addition to the anchoring function provided by the outward radial force of the proximal self-expanding stent member 160 against the inner luminal surface 132 of the patient's vasculature 130 when the stent graft 150 is in a deployed state. The second self-expanding member 202 of the proximal self-expanding stent member 160 may be secured to the proximal end 154 of the main body 152 of the stent graft 150 with one or more struts 168 and/or connector members 216 mechanically coupled to a proximal connector ring 164.

[0060] When loaded on the delivery catheter 100, the first and second self-expanding members 200, 202 of the proximal self-expanding stent member 160 may be radially constrained by releasable belts 104 and 106 which may be releasably held in a constraining configuration by a release member, such as a release wire 120. FIG. 2 shows an embodiment of the proximal self-expanding stent member 160 where the first self-expanding member 200 is being radially constrained by a first releasable belt 104 and the second self-expanding member 202 is being radially constrained by a second releasable belt 106. The first releasable belt 104 may be released by a first release wire 120 and the second releasable belt 106 may be deployed by the second release wire 120. The first and second self-expanding members 200 and 202 of the proximal anchor member may only be released after the outer sheath 102 has been retracted, as shown in FIG. 2, in order to expose the stent graft 150.

[0061] The strut 168 structure of the proximal self-expanding stent member 160 and/or distal self-expanding stent member 170 may be formed from a cylindrical metal tube

structure which is carved or bore by laser or other cutting device. Thereafter, the cut tube may be heat set into two separate forms or states such as an expanded state and non-expanded/contracted state. FIG. 3 shows an example of a non-expanded state. The proximal self-expanding stent member 160 and/or distal self-expanding stent member 170 may include one or more barbs 165. A barb 165 may be any outwardly directed protuberance, typically terminating in a sharp point that is capable of at least partially penetrating a body passageway in which the stent graft 150 is deployed (typically the initial and medial layers of a blood vessel such as the abdominal aorta). The number of barbs 165, the length of each barb 165, each barb 165 angle, and the barb 165 orientation may vary from barb 165 to barb 165 within a single anchor member or between multiple anchor members (i.e., proximal self-expanding stent member 160 and/or distal self-expanding stent member 170) within a single stent graft 150. Although the various barbs 165 (and tuck pads 166, as will be discussed below) may be attached to or fixed on the struts 168, it may be preferred that they are integrally formed as part of the struts 168. When either the proximal self-expanding stent member 160 and/or distal self-expanding stent member 170 is deployed in the abdominal aorta, for example, typically in a location proximal to the aneurysm and any diseased tissue, barbs 165 may be designed to work in conjunction with the distally-oriented blood flow field. In this location, the barbs 165 may penetrate the tissue and prevent axial migration of the stent graft 150. As such, the barbs 165 may be oriented proximally with respect to the main body 152 section. However, the number, dimensions, configuration and orientation of barbs 165 may vary significantly, yet be within the scope of the present invention.

[0062] The staged deployment of the proximal self-expanding stent member 160 may also facilitate self-alignment of the stent graft 150. For instance, upon deployment of the proximal self-expanding stent member 160, the graft may be free to expand and enable distal fluid flow to flow through the stent graft 150 and create a “windsock” effect. That is, the distal fluid flow may apply a slight distal force generally upon the main body 152. This distal force may help to align at least the main body 152 and proximal self-expanding stent member 160 within the patient’s vasculature 130, which may be particularly advantageous during deployment of the stent graft 150 within the angulated vasculature 130, for example.

[0063] In some embodiments of the stent graft 150, one or more struts 168 may include tuck pads 166. Additionally, the one or more struts 168 may have tuck pads 166 positioned such that the tuck pads 166 are generally aligned with a barb 165 extending from an adjacent strut 168, as shown in FIG. 11. As such, during preparation of the stent graft 150 into its reduced diameter delivery configuration (or non-expanded/contracted state), each barb 165 may be placed, for example, behind an adjacent strut 168 and/or tuck pad 166 in order to prevent the barbs 165 from radially extending and contacting the inside of a outer sheath 102 or delivery catheter 100 during delivery of the stent graft 150, as well as to prevent undesired contact of the barbs 165 with the inside luminal surface 132 of a patient’s vasculature 130.

[0064] As illustrated in FIG. 3A, the struts 168 may have various circumferential dimensions and/or cross sectional areas 169. Enlarged portions 180 of a strut 168 may also include varying radial lengths generally along a longitudinal axis of the strut 168. Enlarged portions 180 may be aligned

with barbs 165 and/or located at a generally unstable portion of a strut 168. In some stent graft 150 embodiments, when the stent (i.e., proximal self-expanding member 169) is in a compressed state, enlarged portions 180 may abut each other and may have one or more flat sides which prevent slippage by each other. Adjacent enlarged portions 180 that abut each other and circumferentially interfere with each other may be axially coextensive. In a radially compressed state, for example, the one or more enlarged portions 180 may be compressed to a radial diameter that is no greater than the remaining part of the stent 168.

[0065] In some embodiments, one or more struts 168 may have a tapered section 300. For example, one or more struts 168 may have a tapered section 300 in order to evenly distribute strain induced at least when the stent is in a constrained state. The strut 168 may taper from a first end portion of the strut 168 to a smaller transverse cross section towards a middle portion of the strut 168. As shown in FIG. 7B, a strut 168 embodiment may taper from a proximal end 400 portion towards a respective middle portion 402 and taper to a reduced transverse cross section from a distal end portion 404 towards a respective middle portion 402. The strut 168 may taper over half or approximately half of the length of the strut 168. In addition, the strut 168 may taper generally over the entire length of the strut 168, such as from the apex or crown of the anchor member or stent to the middle of the strut or to the first discontinuity feature (i.e., an enlarged portion 180, barb 165, tuck pad 166 and the like). The struts 168 may taper in at least one transverse dimension of the strut 168. Additionally, the struts 168 may taper along a circumferential direction about the longitudinal axis of the struts 168 may have a substantially constant thickness in a radial direction relative to the longitudinal axis of the stent, such as the proximal self-expanding stent member 160. The struts 168 may taper along a radial direction relative to the longitudinal axis of the anchor member or stent and the struts 168 may have a substantially constant thickness in a circumferential direction about the longitudinal axis of the anchor member or stent. The taper angle of a tapered section 300 of a strut 168 may be about 1 degree to about 3 degrees inclusive, about 1.5 degree to about 2.5 degrees inclusive, or about 1.75 degree to about 2.25 degrees inclusive. The strut 168 embodiments may taper continuously from each end portion to the respective middle portions, such as is shown by way of example in FIG. 9. The struts may include a stepped taper embodiment 302 which tapers in discrete steps rather than a smooth continuous taper from the distal and proximal end portions 404 and 400 of the respective middle portions 402 in either radial direction about the longitudinal axis. Such an embodiment is shown by way of example in FIG. 7C. The struts may also taper in a circumferential direction about the longitudinal axis, as shown in FIG. 8. The tapered sections 300 of the struts 168 may extend from proximal and distal end portions 400 and 404 of the struts 168 to respective strut structures (i.e., enlarged portions 180) disposed in, for example, the middle portion 402 of the respective strut 168, as shown by way of example in FIG. 8.

[0066] FIG. 5 illustrates a portion of a stent 500 embodiment which may function as a proximal self-expanding stent member 160. The stent 500 may include a plurality of struts 168 extending axially between the proximal end 402 and distal end 404 thereof. The stent 500 may be oriented in either direction, depending on the application. Both the

proximal and distal ends **400** and **404** may have a plurality of crowns adjoining adjacent struts **168**. The distal end **404** may have a plurality of connecting members **216** configured to connect the stent **500** to the main body **152** or other structure. The stent **500** embodiment may have various features (i.e., tuck pads **166**, etc.) and structures and is not limited to the strut **168** features and structures illustrated herein. For example, the stent **500** may have a body defined by a lattice structure or a helical structure.

[0067] Optional taper (or tapers) may be incorporated into one or more of the struts **168** of the various stent **500** embodiments, as well as the various connector members **216**. In general, incorporating one or more tapers into one or more of the struts **168** in one or more stents **500** may provide greater space in the tapered section **300** to accommodate alternative features such as barbs **165** and tuck pads **166**. In addition, it may allow for a smaller deployment profile when the components are in a radially collapsed delivery configuration. When configuring the various stents **500** into this reduced diameter delivery profile (non-expanded/constrained state), the stents **500** may experience a large degree of bending strain that may be poorly distributed. Tapering certain stent **500** struts **168** in particular locations may help to distribute this strain more evenly throughout the stent **500** and/or strut **168** which may assist in preventing strain damage to the stent **500**.

[0068] FIG. 5 illustrates a section of a stent **500**, such as a proximal self-expanding stent member **160**, in which the struts **168** taper from a proximal end **400** width to a minimum width about the middle portion **402** of the strut **168**. An example transverse cross-section of the strut **168** taken along line **6AA-6AA**, which is generally located in the proximal end **400** region of a strut **168**, of FIG. 5 is shown in FIG. 6AA (which may or may not equal a width of strut **168** in the apex region or distal end **404**). Another example transverse cross-section of the strut **168** taken along line **6A-6A**, which is generally located in the minimum width, or near the middle portion **402** region of the strut **168**, of FIG. 5 is shown in FIG. 6A. The optional taper, which may be expressed as the taper ratio, is the ratio of the maximum width (as shown, for example, in FIG. 6AA) to the minimum width (as shown in FIG. 6A) of a cross sectional area **169**. The taper ratio may vary widely depending on, for example, the particular region of the strut **168** or connector member **216**, the material used, and other factors. Taper ratios ranging from about 1 to about 10 or greater may be within the scope of the present invention. It may also be within the scope of the present invention for the struts **168** to have no taper (as shown by way of example in FIG. 7A).

[0069] FIGS. 6A-6EE, illustrate a variety of examples of varying transverse cross-sectional views taken at two different locations along a single strut **168**. These figures illustrate examples of the different shapes and sizes a single cross sectional area **169** of a strut **168** may have. For instance, as described above, FIGS. 6A and 6AA show a pair of transverse cross section views of the strut **168** embodiment of FIG. 5 taken along the lines **6A-6A** and **6AA-6AA** which illustrates the rectangular shape of the cross sectional area **169** and the change in size of the cross sectional area **169** at two different locations along the strut **168**. FIGS. 6B and 6BB illustrate another example embodiment of paired transverse cross section views of another strut **168** embodiment which illustrates the trapezoidal shape of the cross sectional area **169** and the change in size of the cross

sectional area **169** at two different locations along the strut **168**. FIGS. 6C and 6CC illustrate another example embodiment of paired transverse cross section views of another strut **168** embodiment which illustrates the inverse trapezoidal shape of the cross sectional area **169** and the change in size of the cross sectional area **169** at two different locations along the strut **168**. FIGS. 6D and 6DD illustrate another example embodiment of paired transverse cross section views of another strut **168** embodiment which illustrates the elliptical shape of the cross sectional area **169** and the change in size of the cross sectional area **169** at two different locations along the strut **168**. FIGS. 6E and 6EE illustrate another example embodiment of paired transverse cross section views of another strut **168** embodiment which illustrates the circular shape of the cross sectional area **169** and the change in size of the cross sectional area **169** at two different locations along the strut **168**. The transverse cross sectional area **169** of one or more locations along a strut **168** are not limited to the sizes and shapes disclosed herein, and may be any number of sizes and shapes that may be incorporated in a strut **168** and/or stent **500** configuration.

[0070] A proximal self-expanding stent member **160** may have, for example, one or more struts **168** having a proximal end **400** portion and/or distal end **404** portion which may be made from NiTi and an effective maximum strut **168** width ranging from about 0.016 to about 0.032 inch; particularly from about 0.022 inch and about 0.028 inch, and a minimum strut **168** width between about 0.010 inch and about 0.026 inch; particularly from about 0.012 inch and about 0.022 inch. Additional tapered strut **168** embodiments are described and shown herein in the figures which may be used in other anchor members (such as the proximal and distal self-expanding stent members **160** and **170**), stent **500** embodiments or connector members **216** described herein, and may be incorporated in any number of components and made from any number of materials. For example, tapering of the struts **168** in any configuration described herein may improve the strain distribution at least between the proximal end **400** portions and distal end **404** portions of the struts **168**.

[0071] Various types of taper features or configurations may be implemented in any number of struts **168** for achieving a variety of strut **168** characteristics. For example, one or more struts **168** may include a taper having an offset radii and/or combinations of elliptical and/or circular apex radii in order to further cause the desired behavior during assembly into a reduced-diameter delivery configuration as well as effective delivery and performance in vivo. For example, the proximal end **400** portion, or apex, width may be the minimum width of the strut **168** which untapers towards the middle portion **402** of the strut **168**, which may have the maximum width of the strut **168**. The tapering from the proximal end **400** portion to the middle portion **402** of the strut **168** may be continuous, stepped in discrete steps **410** with straight untapered portions between each discrete step (as shown by way of example in FIGS. 7C and 8) or a combination thereof. Furthermore, untapering of the strut **168** may be in the radial and/or circumferential direction along the longitudinal length of the strut **168**.

[0072] The strut **168** may include an enlarged portion **180** located in about the middle portion **402** of one or more of the struts **168**, as shown by way of example in FIG. 5. By way of further example, one or more enlarged portions **180** may be located along every other strut **168** of the stent **500**. The

one or more enlarged portion **180** may be located along a strut **168** in various locations, such as near or at the proximal end **400** portion, middle portion **402**, and/or distal end **404** portion of the strut **168**. Additionally, the one or more enlarged portions **180** may be located at offset locations relative to enlarged portions **180** (or other features) along neighboring struts **168**.

[0073] In some cases, the one or more enlarged longitudinal sections or enlarged portions **180** may have an enlarged transverse dimension that is about 1.5 times to about 3 times the nominal transverse dimension of the strut **168** in a direction of the enlargement. Additionally, the enlarged portions **180** may have an undulating configuration of the nominal strut **168**. Furthermore, the enlarged portion **180** may have an oval enlargement of the nominal strut. Each strut **168** of the stent **500** having an enlarged portion **168** along the length of the strut **168** may have only one enlarged portion **180**. Alternatively, each strut **168** of the stent **500** having an enlarged portion **180** along the length of the strut **168** may have more than one enlarged portion **180**. The enlarged portions **180** are not limited to what are described and shown herein, and may be sized, featured, shaped, and proportioned in any number of ways that may assist in assembly or use of the stent **500**. Additionally, any number of materials may be used and may vary between struts **168**, anchor members (such as the proximal and distal self-expanding strut members **160** and **170**), and/or stents **500**.

[0074] FIG. 10A shows an example portion of a cylindrical stent embodiment **500** in a constrained configuration including struts **168** having generally coaxially aligned enlarged portion **180** embodiments having circular or oval features. FIG. 10B shows an example portion of a cylindrical stent embodiment **500** in a constrained configuration having struts **168** with generally coaxially aligned enlarged portion **180** embodiments having square or rectangular features. FIG. 10C shows a portion of a cylindrical stent embodiment **500** in a constrained configuration including struts **168** having undulating deflected portions **182** which may be configured to physically separate adjacent struts **168** in a circumferential direction.

[0075] One or more struts **168** of a stent embodiment **500** may have a stepped taper **302** feature generally along the length of the strut **168**. For example, one or more struts **168** may have a stepped taper **302** from the proximal end **400** to the respective middle portion **402** of the strut **168** and/or a stepped taper **302** from the distal end **404** to the middle portion **402** of the strut **168**, wherein the stepped taper **302** may be in either radial direction about the longitudinal axis of the strut **168**, as shown by way of example in FIG. 7C, or the circumferential direction about the longitudinal axis, as shown by way of example in FIG. 8. The taper characteristics of a strut **168** may be continuous, stepped or any other shape configured to evenly distribute strain induced by the constraint of the constrained non-expanded stent **500**.

[0076] FIG. 7A illustrates an example longitudinal section view taken along line 7A-7A of the strut **168** in FIG. 5 which shows a generally rectangular cross sectional area **169** having no radial tapering about the longitudinal axis. FIG. 7B illustrates another example of a longitudinal section view of a strut **168** which shows a generally tapered cross sectional area **169** due to radial tapering about the longitudinal axis of the strut **168**. In FIG. 7B, the strut **168** tapers continuously from each end portion (the proximal and distal

ends **400** and **404**) to the middle portion **402** such that the middle portion **402** generally has the minimum strut **168** width in the radial direction. FIG. 7C shows another example strut **168** embodiment in longitudinal section including a radial stepped tapering **302** about the longitudinal axis of the strut **168**. In FIG. 7C, the strut **168** generally tapers in steps continuously from each end portion (the proximal and distal ends **400** and **404**) to the middle portion **402** such that the middle portion **402** generally has the minimum strut **168** width in the radial direction.

[0077] FIG. 8 shows a portion of an embodiment of a stent **500** including struts **168** having a circumferential stepped taper **302** configuration about the longitudinal axis of the strut **168**. The middle portion **402** of each strut **168** may also include an enlarged portion **180** extending, for example, in a circumferential direction. Portions of the stepped taper **302** of a strut **168** that may be directly adjacent an enlarged portion **180** may have the minimum strut **168** width in the circumferential direction. However, any number of combinations of tapering in any direction may be used.

[0078] FIG. 9 shows a stent embodiment **500** where the proximal self-expanding stent member **160** has a first self-expanding member **200** secured to a second self-expanding member **202** where the first self-expanding member **200** has alternating more proximally placed barbs **165** along the struts **168** with more distally placed barbs **165** along the struts **168**. In addition, the stent embodiment **500** may have a continuous taper in the second self-expanding member **202**, which is the portion of the proximal self-expanding stent member **160** adjacent the main body **152**. Each strut **168** on the first self-expanding member **168** may have a barb **165** in a different location relative to a neighboring strut **168**. The barbs **165** may be formed integrally with the struts **168**, but may otherwise be manufactured, for example, as a separate component attached to the struts **168**. In general, the struts **168** and the barbs **165** of the stent embodiments **500** and anchor members may be self-expanding, that is, upon release of a constraining force, the struts **168** may move radially apart and the barbs **165** may extend radially outward. Other configurations, such as balloon expansion, are also contemplated within the present invention.

[0079] In addition, stent embodiments **500** may include struts **168** including tuck pads **166**, which may be positioned along a strut **168** such that the tuck pads **166** are axially aligned with a barb **165** positioned on a neighboring strut **168**. Similar to the barbs **165** and enlarged portions **180**, the number, dimensions, configurations and orientations of the tuck pads **166** may vary between struts **168**, stent embodiments **500** and anchor members (such as the proximal and distal self-expanding stent members **160** and **170** described herein).

[0080] During preparation of a stent graft embodiment **150** (and therefore one or more proximal self-expanding stent members **160**) into a reduced diameter delivery configuration, one or more barbs **165** may be placed behind a corresponding strut **168** and/or tuck pad **166**, if present, in order to prevent the barbs **165** from contacting the inside of a outer sheath **102** or delivery catheter **100** during delivery of the stent graft **150** and from undesired contact with the interior luminal surface **132** of the patient's vasculature **130**. As described in copending U.S. patent application Ser. No. 09/917,371 to Chobotov et al., now U.S. Pat. No. 6,761,733, and which is incorporated by reference herein in its entirety, a release belt may be disposed in one or more grooves (not

shown) disposed on one or more struts **168** which may assist in retaining the proximal self-expanding stent member **160** in the reduced diameter delivery configuration.

[0081] For example, upon deployment of stent graft **150**, and more particularly the proximal self-expanding stent member **160**, (typically accomplished, at least in part, by release of one or more belts, such as the proximal releasable belts **104** and **106**), the radial expansion of the proximal self-expanding stent member **160** results in a displacement of struts **168** so that the distance between them increases. Eventually, the displacement between the struts **168** become large enough to enable the barbs **165** to be released from behind the adjacent strut **168** and/or tuck pad **166** and engage the interior luminal surface **132** of the patient's vasculature **130**. In general, the barbs **165** may release into a position suitable for engaging the interior luminal surface **132** of a patient's vasculature with a time constant that is generally an order of magnitude lower than the time constant associated with the radial expansion of the stent **500** embodiment or anchor member (such as the proximal self-expanding stent member **160**). In other words, during the stent **500** or anchor member deployment process, the one or more barbs **165** may complete their deployment before the stent **500** or anchor member is fully expanded so that the barbs **165** may engage the interior luminal surface **132** of the vasculature **130** with maximum effectiveness.

[0082] Referring again to FIG. 9, the proximal self-expanding stent member **160** may include struts **168**, any one of which may further comprise one or more barbs **165**. In addition, optional tuck pads **166** may be positioned along a strut **168** such that the tuck pad **166** is coaxially aligned with a barb **165** on a neighboring strut **168** in order to shield the neighboring barb **165** at least when the stent graft **150** is in its reduced diameter delivery configuration. Struts **168** and/or tuck pads **166** may also include a tuck slot **167** which may assist in retaining a barb **165** while the stent graft **150** (and consequently the proximal self-expanding stent member **160**) is in its reduced diameter delivery configuration. Upon deployment of a stent graft **150** embodiment, the one or more barbs **165** may be released from respective tuck slots **167** and thereafter placed in an operational or deployed configuration for engaging a patient's vasculature **130**.

[0083] FIG. 11 shows a portion of a cylindrical stent embodiment **500** in a generally constrained and flattened configuration having struts **168** with a coaxial enlarged portion **180** embodiments and undulating deflected portions **182**. The undulating deflected portions **182** may have barbs **165** positioned at offset proximal and distal locations along neighboring struts **168** which may aid in efficiently compacting the struts **168** and barbs **165** in a constrained configuration for delivery into a patient's body. By alternating axial location of the barbs **165** and/or enlarged portions **180** along neighboring struts **168**, the stent **500** may be optimally compressed. The undulating deflected portions **182** of a strut **168** may enable multiple lateral contact points within the stent **500**. Such multiple contact points may aid in restraining or compacting the stent **500** in a constrained/non-expanded state. In some embodiments, one or more struts **168** may have enlarged longitudinal sections or enlarged portions **180** that may be disposed in a substantially longitudinal orientation between the proximal end and distal end of the stent **500** when the stent **500** is in the constrained state. Additionally, the one or more struts **168** may be disposed in an undulating pattern. FIG. 12 shows a trans-

verse cross section view of the stent **500** portion of FIG. 11 taken along lines 12-12 of FIG. 11. FIG. 12 illustrates an example of the varying circumferential cross sectional areas **169** of the struts **168** taken along a transverse cross section of the strut **500**.

[0084] As discussed above, some embodiments of a modular endovascular stent graft assembly may include a bifurcated graft member **600** with a proximal stent or anchor member **602** secured thereto. In some cases, the main body member **604** may be formed from a supple graft material, such as ePTFE, having a main fluid flow lumen **606** therein. FIG. 13 illustrates such an embodiment. Referring to this figure, the main graft portion **604** may include an ipsilateral leg **608** with an ipsilateral fluid flow lumen **610** in communication with the main fluid flow lumen **606**, a contralateral leg **612** with a contralateral fluid flow lumen **614** in communication with the main fluid flow lumen **606** and a network of inflatable channels **616** disposed on the main graft member **604**. For some embodiments, the main graft or main body member **604** may have an axial length of about 5 cm to about 10 cm, more specifically, about 6 cm to about 8 cm in order to span an aneurysm **622** of a patient's aorta **618** without engaging the patient's iliac arteries **620** directly with the legs **608** and **612** of the main graft member **604** (see FIG. 14).

[0085] The inflatable channels of the network of inflatable channels **616** may be disposed on any portion of the main graft or main body member **604** including the ipsilateral and contralateral legs **608** and **612**. The network of inflatable channels **616** may be configured to accept a hardenable fill material to provide structural rigidity to the main body **604** member when the network of inflatable channels **616** are in an inflated state and the inflation material has been cured or hardened. Radiopaque inflation material may be used to facilitate monitoring of the fill process and subsequent engagement of graft extensions. The network of inflatable channels **616** may also include at least one inflatable cuff **624** disposed on a proximal portion of the main body member which may be configured to seal against an inside surface of a patient's vessel, such as the aorta.

[0086] The proximal anchor member **626**, which may have a substantially tubular or cylindrical configuration, may be disposed at a proximal end **628** of the main body member **604** and secured to the main body member **604** in any suitable manner including stitching, adhesive bonding, welding, and the like. The proximal anchor member **626** may also be secured to the main body **604** with a resilient connector ring (not shown) which may be embedded in a proximal end or portion **628** the main body **604**. The proximal anchor member **626** may have a self-expanding proximal stent portion **630** secured to a self-expanding distal stent portion **632**. Each of these stent portions **630** and **632** may include an undulating elongate stent element that may be disposed in a somewhat serpentine or sinusoidal configuration, as shown above with regard to stent members **160** and **170**. Each of the stent portions **630** and **632** of the proximal anchor member **626** of the stent graft **600** in FIG. 13 may share any or all of the features, dimensions or materials of stent members **160** and **170** discussed above. For example, the proximal and distal stent portions **630** and **632** of the proximal anchor member **626** may include tapered struts **634** that extend between crown portions **636** of each respective stent portion **630** or **632**. Such tapered struts **634** may have any or all of the features, dimensions,

and materials of the struts discussed above and include a tapered strut configuration that allows for the strain imposed on the strut structure to be evenly distributed through the structure of the stent portion or portions 630 and 632.

[0087] In some cases, the proximal stent portion 630 may be secured to the distal stent portion 632 with one or more struts or strut segments 638 disposed between the respective proximal and distal stent sections 630 and 632. Some embodiments of such interconnecting struts 638 may have a cross sectional area that is substantially the same as or greater than a cross sectional area of proximal stent portions 630 or distal stent portions 632 adjacent the strut 638. Such configurations may be useful in avoiding points of concentrated stress in the proximal anchor member 602 or struts 638 which couple components thereof. For some embodiments, the proximal stent portion 630 of the proximal anchor member 602 may further include a plurality of barbs 640 having sharp tissue engaging tips 642 that are configured to extend in a radial outward direction in a deployed expanded state (see FIG. 15). For some embodiments, each stent portion 630 and 632 of the proximal anchor member 602 may include about 5 crowns 636 to about 8 crowns 636 at either end of the respective section 630 or 632 and may be made from a superelastic alloy such as superelastic NiTi alloy.

[0088] At least one tubular ipsilateral graft extension 644 having a fluid flow lumen 646 disposed therein may be deployed with the fluid flow lumen 646 of the graft extension 644 sealed to and in fluid communication with the fluid flow lumen 610 of the ipsilateral leg 608 of the main body member 604. In addition, at least one tubular contralateral graft extension 648 having a fluid flow lumen 650 disposed therein may be deployed with the fluid flow lumen 650 of the graft extension 648 sealed to and in fluid communication with the fluid flow lumen 614 of the contralateral leg 612 of the main body member 604. For some embodiments, the graft extensions 644 and 648 may include an interposed self-expanding stent 652 disposed between at least one outer layer and at least one inner layer of supple layers of graft material. The interposed stent disposed between the outer layer and inner layer of graft material may be formed from an elongate resilient element helically wound with a plurality of longitudinally spaced turns into an open tubular configuration. For some embodiments, the interposed stent 652 may include a superelastic alloy such as superelastic NiTi alloy. In addition, the graft material of each graft extension 644 and 648 may further include at least one axial zone of low permeability for some embodiments.

[0089] For some embodiments, an outside surface of the graft extension 648 may be sealed to an inside surface of the contralateral leg 612 of the main body 604 when the graft extension 648 is in a deployed state. For some embodiments, the axial length of the ipsilateral and contralateral legs 608 and 612 may be sufficient to provide adequate surface area contact with outer surfaces of graft extensions 644 and 648 to provide sufficient friction to hold the graft extensions 644 and 648 in place. For some embodiments, the ipsilateral and contralateral legs 608 and 612 may have an axial length of at least about 2 cm. For some embodiments, the ipsilateral and contralateral legs 608 and 612 may have an axial length of about 2 cm to about 6 cm, more specifically, about 3 cm to about 5 cm.

[0090] For the bifurcated stent graft embodiment 600 discussed above or any other suitable stent graft embodi-

ment discussed herein that includes a proximal self-expanding anchor member 602, it may be desirable in some cases to constrain each of the proximal and distal stent portions 630 and 632 separately so that each of the proximal and distal stent portions 630 and 632 of the proximal anchor member 602 can be deployed from a radially constrained state independent of each other. FIG. 14 shows the stent graft 600 having an 8 crown distal stent portion 632 with marker elements 654 disposed at a distal end 656 of the distal stent portion 632. Other than this variation in the proximal anchor configuration, the stent graft of FIG. 14 may have the same features, dimensions and materials as those of the stent graft 600 shown in FIG. 13.

[0091] The stent graft 600 of FIG. 14 is shown in a partially deployed state within an abdominal aorta 618 of a patient with the proximal end 628 of the main body 604 disposed just below and in a non-interfering relationship with the renal arteries 658 which extend from and are in communication with the patient's aorta. The main body 604 of the stent graft 600 also extends substantially across the aneurysm 622 of the aorta 618, however, this relationship may vary depending on the size of the graft 600 used and the morphology of the aneurysm 632. The proximal stent portion 630 of the proximal anchor member 602 is still constrained by a releasable member or belt 660 such that it has an outer dimension or profile suitable for delivery within a catheter assembly within the patient's vasculature. The distal stent portion 632, however, has been released from a constrained state and has expanded radially such that the distal end 656 of the distal stent portion 632 has expanded outwardly in approximation to the inner surface 662 of the patient's aorta 618.

[0092] In such cases, a proximal anchor member 602 configured to allow the distal end 656 of the distal stent portion 632 to so expand may be desirable. For example, the markers 654 disposed at the distal end 656 of the distal stent portion 632 are substantially open and are close to or in contact with the inner wall 662 of the patient's aorta 68 providing good visualization of the position of the partially deployed stent graft 600 under fluoroscopy. This configuration may allow the physician deploying the stent graft 600 to visualize the position of the stent graft 600 and accurately predict what the final position of the stent graft 600 will be after complete deployment. However, such a configuration may also allow the physician to adjust the position of the stent graft 600 prior to full deployment of the proximal anchor member 602. In other words, the stent graft 600 and markers 654 at the distal end 656 of the distal stent portion 632 are sufficiently expanded so that the physician can easily see how the stent graft 600 will be positioned when fully deployed before the physician has deployed the proximal stent portion 630 in which case the barbs 640 or other tissue engaging members of the proximal stent portion 630 engage the tissue of the inner wall 662 of the patient's aorta 618.

[0093] We have found that in some instances, in order to configure an anchor member 602 such that the distal end 656 of the distal stent portion 632 opens or radially expands sufficiently upon release from a constrained state, that certain design parameters or criteria may be desirable. In particular, such a stent portion 632 may benefit from a configuration that produces a good distal opening force or maximum opening force in an outward radial direction. In order to produce a generous opening force in an outward radial direction, the section of the struts 634 and crowns 636

of the proximal and distal stent portions 630 and 632 may be increased, however, it may also be desirable to adjust the tapering profile of the struts 634 in order to maintain a substantially even distribution of strain throughout the structure of the stent portions 630 and 632. For some embodiments, a useful outward opening force may include about 0.5 to about 0.75 lbf of force for a stent embodiment that is about 14 mm to about 16 mm in outer diameter in a relaxed unconstrained state.

[0094] In cases such as the stent graft embodiment 600 of FIG. 13 wherein the proximal anchor member 602 includes both a proximal stent portion 630 and a distal stent portion 632, it may be useful to vary the axial lengths of the respective proximal and distal portions 630 and 632 of the anchor member 602. Such an unsymmetric arrangement may be beneficial in cases such as the partial deployment sequence step shown in FIG. 14 wherein the constraint on the distal stent portion 632 has been released so as to allow radial expansion of the distal portion 632 but the proximal stent portion 630 remains constrained.

[0095] FIG. 15 illustrates an embodiment of the proximal anchor member 602 having a 5 crown proximal stent portion 630 and a five crown distal stent portion 632. An attachment ring 664 is secured to each crown 636 of the distal end 656 of the distal stent portion 632. Such attachment rings 664 may be secured to the proximal end 628 of main body 604 by stitching the ring 664 to the flexible material of the main body portion 604 with suture or any other suitable material. Such attachment rings 664 may also be secured to the main body 604 by any other suitable method including any of the attachment methods and devices discussed above. A cutaway portion 668 of the proximal anchor member 602 is shown at the ends of arrows 665 to illustrate an element of the proximal anchor member 602 for further discussion. The cutaway portion 668 includes a distal crown 670 and respective stent struts 634 attached thereto from the distal stent portion 632 and a proximal crown 672 and respective stent struts 634 attached thereto from the proximal stent portion 630. The proximal end of the distal stent portion 632 is secured to the distal end 676 of the proximal stent portion 630 by strut segments 638.

[0096] FIG. 16 illustrates the cutaway portion 668 of the proximal anchor member 602 of FIG. 15 with an adjacent arrow 678 that indicates the axial length of the proximal stent portion 630 and an arrow 680 that indicates the axial length of the proximal stent portion 630 together with the distal stent portion 632 or, in other words, the axial length of the proximal anchor member 602 as a whole. For some embodiments, it has been determined that one or more of the design parameters discussed above may be optimized by use of a proximal anchor member 602 having a proximal stent portion 630 and a distal stent portion 632 wherein the axial length of the proximal anchor member 602 as a whole (L_{stent}) divided by the axial length of the proximal stent portion 630 ($L_{proximal}$) is a ratio of about 1.75 to about 2.5, more specifically, about 1.75 to about 2.1, and even more specifically, about 1.75 to about 1.9. Such a configuration may be useful for a multi-element stent or proximal anchor member 602 in order to maximize opening force and minimize peak strain within the proximal anchor member 602.

[0097] It has also been discovered that for such proximal anchor member embodiments 600 as shown in FIG. 16 including unsymmetric axial lengths of the proximal stent portion 630 and distal stent portion 632, that it may also be

useful to include unsymmetric taper lengths. FIG. 17 illustrates the cutaway portion 668 of the proximal anchor member 602 of FIG. 15 with an arrow 682 that indicates the axial length of the tapered portion 684 of the strut 634 that tapers from the proximal end 674 of the distal stent portion 632 towards the distal end 656 of the distal stent portion 632. Such a tapered portion 684 extends from the crown 686 of the distal stent portion 632 at a proximal end thereof to an axial position of minimum strut cross section 688 between the proximal crown 686 and distal crown 670 of the distal stent portion 632. Distal of the position of minimum section 688 on the strut 634, the strut 634 may begin to flare and increase in section towards the distal crown 670. Thus, the point of minimum section 688 on the strut 634 represents the endpoint of the tapered portions 684 of the strut 634 which begin at each respective crown 670 and 686 of the distal stent portion 632. For some stent embodiments 602, a strut taper configuration wherein the axial length of the proximal anchor member as a whole 602 or L_{stent} divided by the axial length of the tapered strut 634 from the crown 686 of the distal stent portion 632 at a proximal end 674 thereof to an axial position of minimum strut cross section 688 between the proximal crown 686 and distal crown 670 of the distal stent portion 632 (L_{taper}) is about 3.0 to about 4.5, may be particularly useful in order to maximize opening force and reduce or minimize peak strains within the structure of the proximal anchor member 602. It should also be noted that such unsymmetric taper lengths may also be used for multi-element stents or proximal anchor members 602 having stent portions 630 and 632 of equal axial length.

[0098] Another design parameter that may be useful when maximizing opening force and minimizing peak strain within a proximal anchor member 602 is selection of the inner crown radius of the crowns 636 at each end of the respective proximal and distal stent portions 630 and 632. FIGS. 18 and 19 illustrate an inner crown radius R of a distal crown 670 of the distal stent portion 632 of the proximal anchor member 602. For some embodiments, it may be useful to have an inner crown radius R of about 0.001 inches to about 0.005 inches, more specifically, about 0.001 inches to about 0.004 inches. It should be noted that such inner crown radii dimensions R may also be used for single element stents or proximal anchor members 160 and 170, particularly in embodiments where it is desirable to maximize opening force and minimize peak strains within the proximal anchor member.

[0099] For some particular stent graft embodiments 600 having a bifurcated main body 604 and a multi-element proximal anchor member 602, the proximal anchor member 602 may be configured to open to a maximum diameter of about 29 mm to about 31 mm, more specifically, about 30 mm, the proximal anchor member may have an overall axial length L_{stent} of about 35 mm to about 37 mm, more specifically, about 36 mm, an opening force of about 0.5 lbf to about 0.7 lbf, more specifically, about 0.6 lbf, and a ratio of the axial length 680 of the anchor member 602 L_{stent} divided by the axial length 678 of the proximal stent portion 630 $L_{proximal}$ of about 2.0 to about 2.2, more specifically, about 2.1. Such an embodiment 600 may also have a distal stent portion 632 with a strut taper configuration wherein the length 680 of the proximal anchor member 602 as a whole L_{stent} divided by the length 682 of the tapered strut 639 from the crown 686 of the distal stent portion 632 at a proximal end thereof to an axial position of minimum strut cross

section **688** between the proximal crown **686** and distal crown **670** of the distal stent portion **632** (L_{taper}) is about 3.0 to about 3.2, more specifically, about 3.1. Many other embodiments following the design parameters discussed above may also be used in order to maximize opening force and minimize peak strain within the proximal anchor member **602**. As discussed above, these design parameters may also be used singly or in any combination in order to achieve the desired results in either single element stents **160** and **170** or multi-element stents **600** having a proximal stent portion **630**, distal stent portion **632** or any other number of stent portions.

[0100] While preferred embodiments of the invention have been shown and described herein, it will be understood that such embodiments are provided by way of example only. Numerous variations, changes and substitutions will occur to those skilled in the art without departing from the spirit of the invention. Accordingly, it is intended that the appended claims cover all such variations as fall within the spirit and scope of the invention.

[0101] The number of barbs, enlarged portions or tapers per strut, the length of each barb, enlarged portions or tapers, each of the barb angles or tapered angle described above, and the barb, enlarged portion or tapered orientation may vary from barb to barb, enlarged portion to enlarged portion, strut to strut within a single stent or between multiple stents within a single graft.

[0102] The entirety of each patent, patent application, publication and document referenced herein hereby is incorporated by reference. Citation of the above patents, patent applications, publications and documents is not an admission that any of the foregoing is pertinent prior art, nor does it constitute any admission as to the contents or date of these publications or documents.

[0103] Modifications may be made to the foregoing without departing from the basic aspects of the invention. Although embodiments of the invention have been described in substantial detail with reference to one or more specific embodiments, those of ordinary skill in the art will recognize that changes may be made to the embodiments specifically disclosed in this application, yet these modifications and improvements are within the scope and spirit of the invention.

[0104] Embodiments illustratively described herein suitably may be practiced in the absence of any element(s) not specifically disclosed herein. Thus, for example, in each instance herein any of the terms “comprising,” “consisting essentially of,” and “consisting of” may be replaced with either of the other two terms. The terms and expressions which have been employed are used as terms of description and not of limitation and use of such terms and expressions do not exclude any equivalents of the features shown and described or portions thereof and various modifications are possible within the scope of the invention claimed. The term “a” or “an” can refer to one or a plurality of the elements it modifies (e.g., “a reagent” can mean one or more reagents) unless it is contextually clear either one of the elements or more than one of the elements is described. Thus, it should be understood that although embodiments have been specifically disclosed by representative embodiments and optional features, modification and variation of the concepts herein disclosed may be resorted to by those skilled in the art, and such modifications and variations are considered within the scope of this invention.

[0105] Certain embodiments of the invention are set forth in the claim(s) that follow(s).

1-30. (canceled)

31. A self-expanding cylindrical stent having a constrained state and a relaxed expanded state, comprising:

- a proximal end;
- a distal end; and
- a plurality of first resilient struts configured to exert an outward radial force in the constrained state, each of the plurality of first resilient struts comprising an enlarged longitudinal section which is enlarged in a circumferential orientation relative to a longitudinal axis of the stent and configured to stabilize the plurality of first resilient struts, wherein the enlarged longitudinal sections of two adjacent resilient struts of the plurality of first resilient struts contact each other in the constraint state.

32. The stent of claim **31**, wherein the enlarged longitudinal section of a first resilient strut of the plurality of first resilient struts contacts the enlarged longitudinal sections of two second resilient struts of the plurality of resilient struts in the constraint state.

33. The stent of claim **31**, wherein the enlarged longitudinal section of one of the plurality of first resilient struts comprises one or more flat sides.

34. The stent of claim **31**, wherein the enlarged longitudinal sections of the two adjacent resilient struts circumferentially interfere with each other as the enlarged longitudinal sections of the two adjacent resilient struts contact each other in the constraint state.

35. The stent of claim **31**, wherein the enlarged longitudinal sections of the two adjacent resilient struts are axially coextensive.

36. The stent of claim **31**, wherein in the constraint state, the enlarged longitudinal sections of the plurality of first resilient struts are compressed to a radial diameter that is no greater than a radial diameter of a remaining part of the stent.

37. The stent of claim **31**, further comprising a plurality of second resilient struts configured to exert an outward radial force in the constrained state, each of the plurality of second resilient struts comprising a body and a barbed section that extends from the body.

38. The stent of claim **37**, wherein locations and orientations of the barbed sections of two adjacent resilient struts of the plurality of second resilient struts are asymmetric about a dimension that extends across the plurality of second resilient struts.

39. The stent of claim **37**, wherein each of the plurality of second resilient struts comprises a section, wherein the barbed section has a first flat surface, and the enlarged section comprises a second flat surface.

40. The stent of claim **39**, wherein a first flat surface of a first resilient strut of the plurality of second resilient struts faces a second flat surface of a second resilient strut of the plurality of second resilient struts.

41. The stent of claim **37**, wherein locations of the barbed sections of the plurality of second resilient struts are alternating across the plurality of second resilient struts.

42. The stent of claim **37**, wherein one of the plurality of first resilient struts is adjacent to one of the plurality of second resilient struts.

43. The stent of claim **31**, wherein the plurality of first resilient struts do not comprise barbed portion.

44. The stent of claim **31**, wherein a transverse dimension of the enlarged longitudinal section of one of the plurality of first resilient struts is 1.5 times to 3 times a nominal transverse dimension of the one of the plurality of first resilient struts in the circumferential orientation.

45. The stent of claim **31**, wherein each of the plurality of first resilient struts comprises two or more of the enlarged longitudinal sections; each of the plurality of first resilient struts comprises only one of the enlarged longitudinal section.

46. The stent of claim **31**, wherein a location of the enlarged longitudinal section of a first one of the two adjacent resilient struts of the plurality of first resilient struts is offset from a location of the enlarged longitudinal section of a second one of the two adjacent resilient struts of the plurality of first resilient struts, along an axial dimension of the two adjacent resilient struts.

47. The stent of claim **31**, wherein a cross-section of a body of one of the plurality of first resilient struts has a trapezoidal shape.

48. The stent of claim **31**, wherein a cross-section of a body of one of the plurality of first resilient struts has an oval or round shape.

49. The stent of claim **31**, wherein a cross-section of a body of one of the two adjacent resilient struts and a cross-section of a body of another one of the two adjacent resilient struts are complementary.

50. The stent of claim **31**, wherein at least one of the plurality of first resilient struts comprises a taper having an offset radius, an elliptical apex radius, or a circular apex radius.

* * * * *