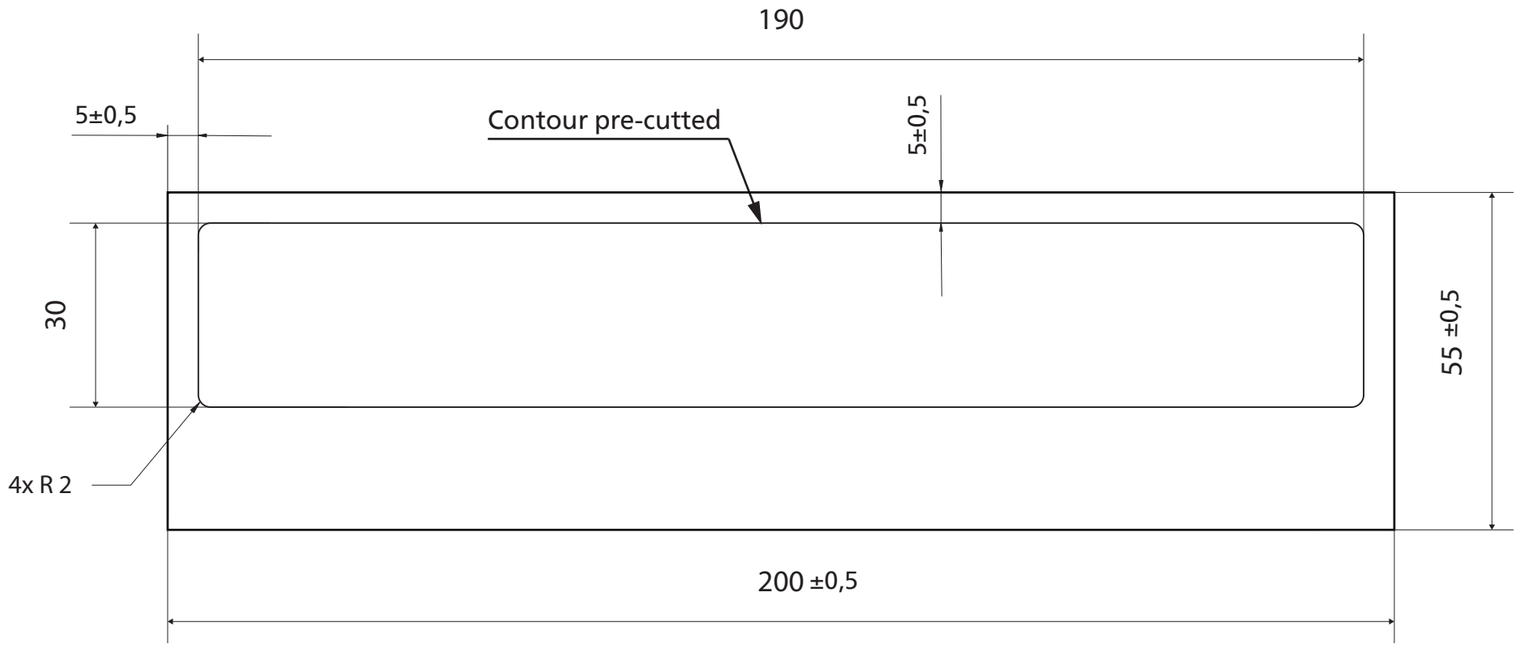

-	-	-	-
-	-	-	-
-	-	-	-
-	-	-	-
2609	As issued	24-FEB-2026	Viktor Weidmann
DWG.- REV.	REVISION DESCRIPTION	DATE	APPROVED

NOTES:

1 - CONTROL DIMENSION

2 - NOMINAL GEOMETRY DATA IS DEFINED IN ASSOCIATED CAD-DATA FILE

3 - FOR ALL FURTHER INFORMATION SEE SPECIFICATION DOCUMENT

4 - TOL MARKED DIMENSIONS ARE USED BY PHILIPS WITHIN TOLERANCE ANALYSIS

5 - DIMENSIONS/PROPERTIES INCLUDING THE SUFFIX CTQ ARE CRITICAL TO QUALITY
DIMENSIONS/PROPERTIES INCLUDING THE SUFFIX CTS ARE CRITICAL TO SAFETY

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN MILLIMETRES

FIRST ANGLE
PROJECTION

DO NOT SCALE THIS DRAWING

TOLERANCES
ISO 8015:2011 (AD) -
MEASURING TEMPERATURE 22°C ± 3K
AIR HUMIDITY 50% ± 10%

GENERAL TOLERANCE PER DIN EN ISO 22081:
LINEAR SIZES (for label sizes and label to label distances): DIN 2769-b
LINEAR SIZES (for sheet outline and labelset on sheet): DIN 2769-c
ANGULAR SIZES: DIN 2769-2
RADII: ±0,3mm

	DATE	NAME
DRAWN	24-FEB-2026	Viktor Weidmann
CHECKED		

SCALE 1:1

PAPER SIZE A3

TITLE

LBL 190x30mm blanko

DRAWING NUMBER 453665226081-M-ADWG

SHEET 1/1

- STRENG VERTRAULICH -
WEITERGABE AN DRITTE UND VERVIELFÄLTIGUNGEN NUR MIT GENEHMIGUNG DES URHEBERS
SCHUTZVERMERK NACH ISO 16016 BEACHTEN

PHILIPS MEDICAL SYSTEMS PROPRIETARY
This document contains confidential proprietary information that is PHILIPS PROPRIETARY.
Do not disclose to or duplicate for others except as authorized by PHILIPS MEDICAL SYSTEMS.

PHILIPS