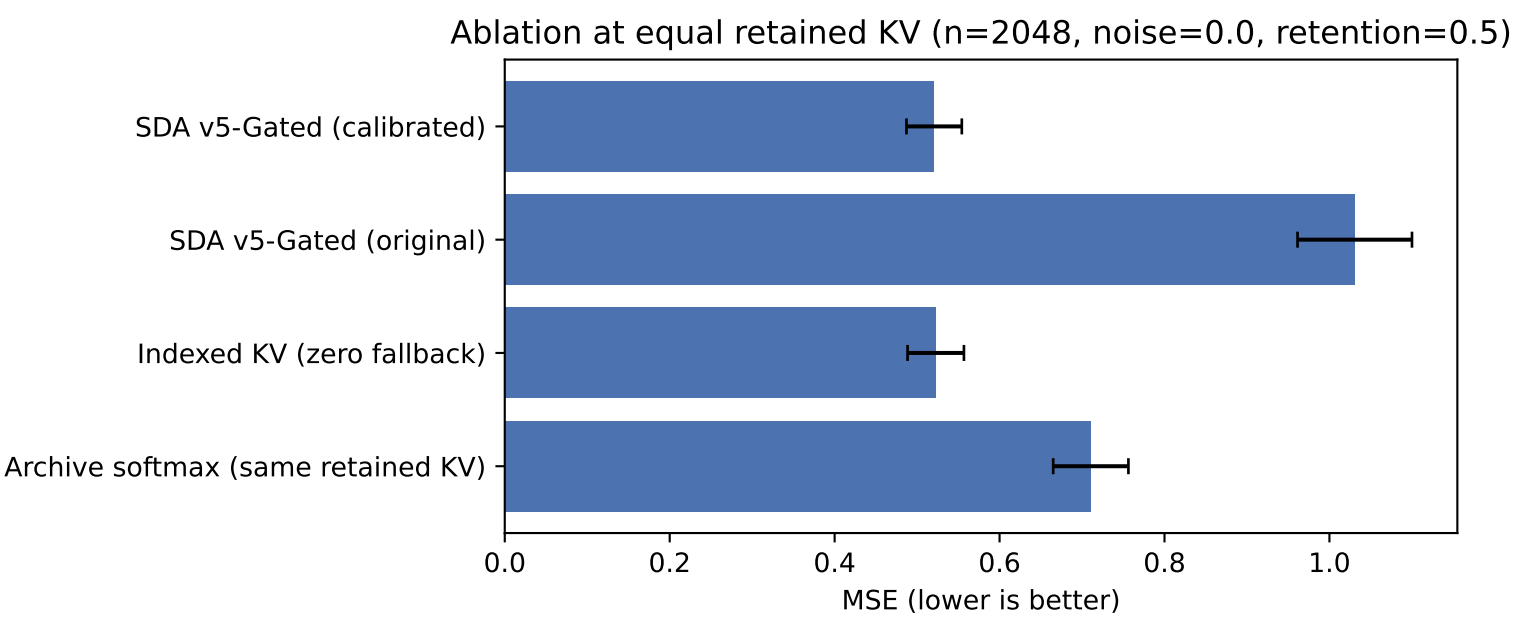
Ablation at equal retained KV (n=2048, noise=0.0, retention=0.5)
SDA v5-Gated (calibrated)
SDA v5-Gated (original)
Indexed KV (zero fallback)
Archive softmax (same retained KV)
0.0
0.2
0.4
0.6
0.8
1.0
MSE (lower is better)