



Mayura Analytical LLP

Yelachenahalli, Bangalore - 70

User Name : a

Instrument Id : 123456

Date : 2022-06-19

Time : 09:54:10 PM

Method File : pot1

Batch Number : 1

AR Number : 1

Sample Name: 1

Dosage Speed : 4.0

EP Select : Auto

No. of Trials : 2

Titrant Name : 1

Normality : 1.0

Formula No. : 1


Trial No	V1 mL	Wt/gm	Moisture	Normality
1	1.403	10.0	1.0	7.055
2	1.346	10.0	1.0	7.357

Remarks : No remarks

a
Analyzed By

Certified By

Potentiometry

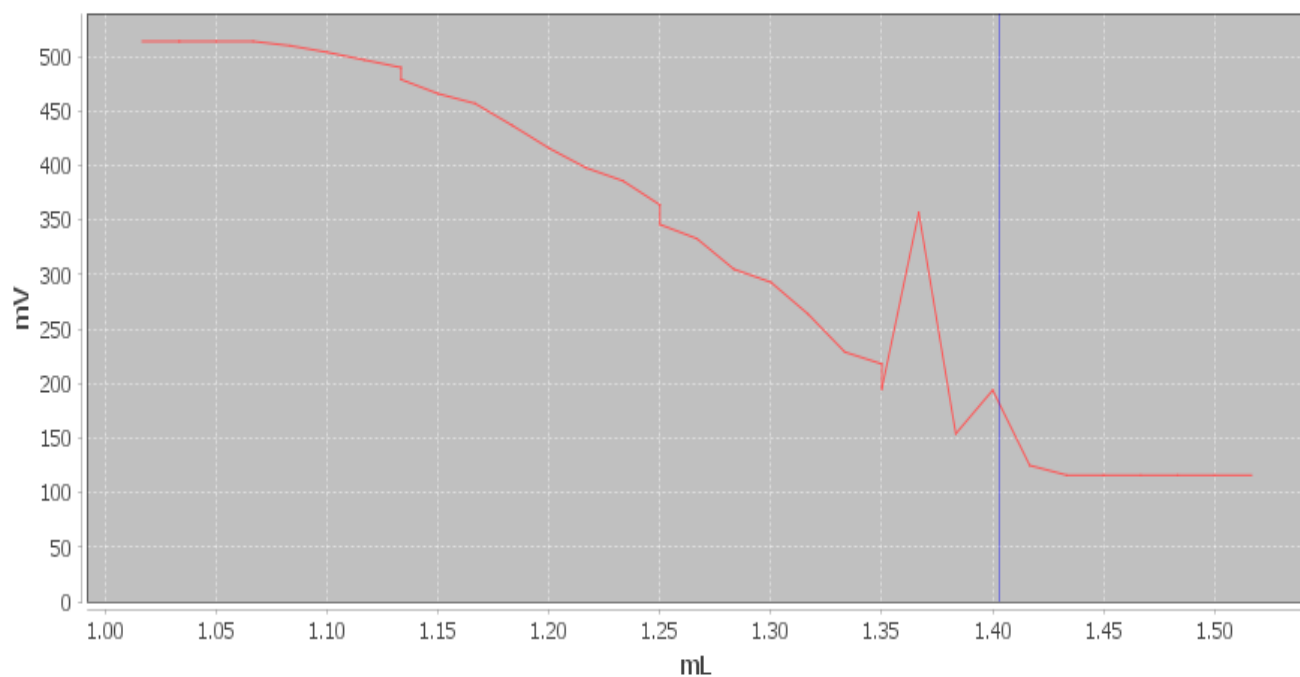

Date : 2022-06-19

Time: 09:54:13 PM

Stir Time: 2.0

Pre-Dose: 1.0

Method File: pot1

Trial No.: 1

Dosage Speed: 4.0

Threshold: 100

End Point: Auto


Report Name: 1h

Trial No	V1 mL	Wt/gm	Moisture	Normality
1	1.403	10.0	1.0	7.055

a
Analyzed By

Certified By

Potentiometry

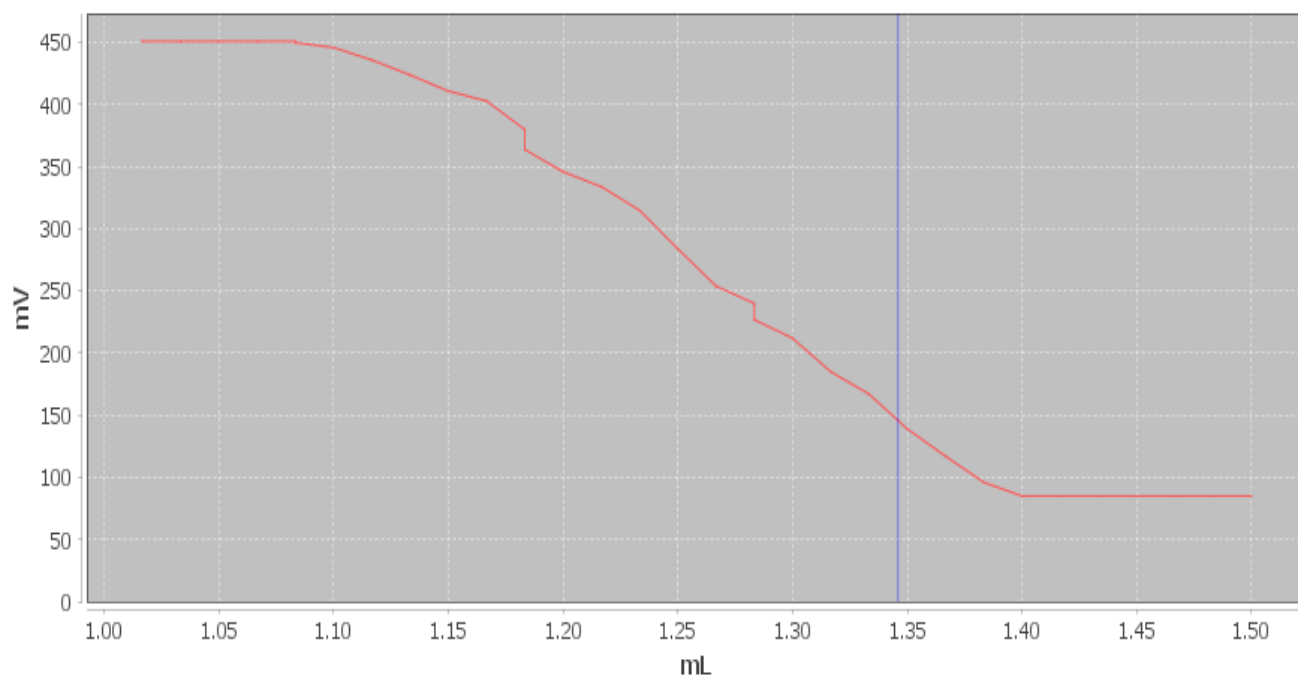

Date : 2022-06-19

Time: 09:54:41 PM

Stir Time: 2.0

Pre-Dose: 1.0

Method File: pot1

Trial No.: 2

Dosage Speed: 4.0

Threshold: 100

End Point: Auto

Report Name: 1h

Trial No	V1 mL	Wt/gm	Moisture	Normality
2	1.346	10.0	1.0	7.357

a
Analyzed By

Certified By