


Ablation: contribution of each component to defect detection

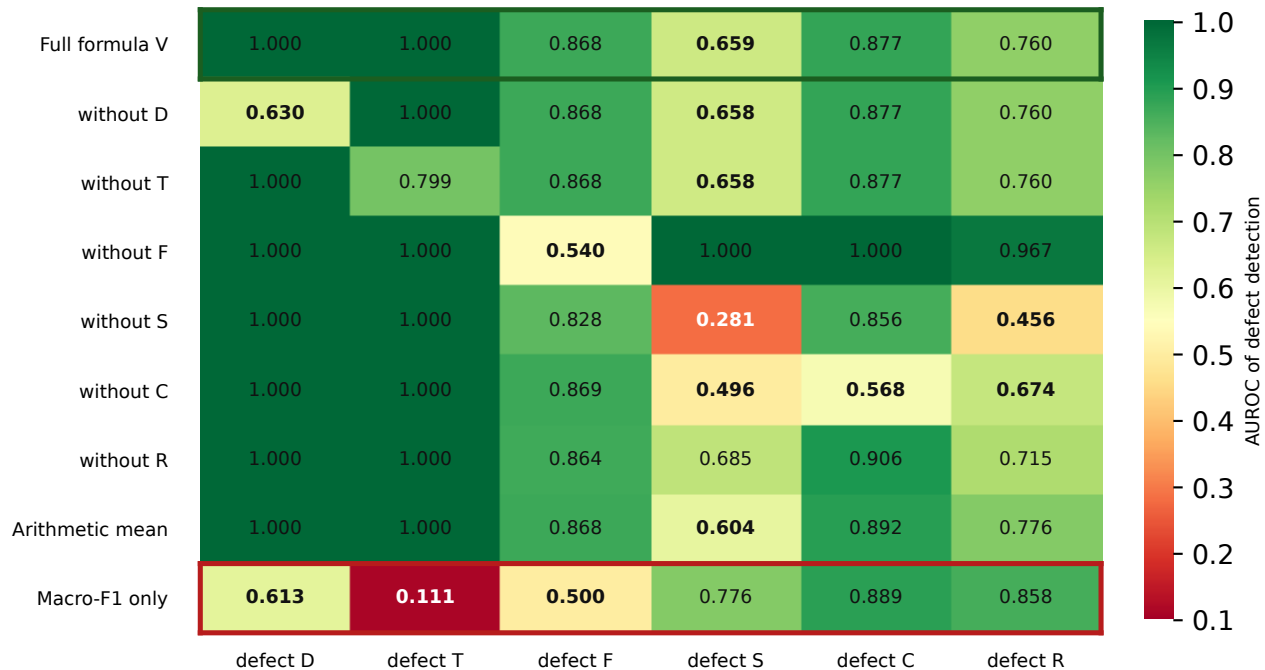

Removing a component collapses the detection of its corresponding defect. Bottom row: macro-F1 yields AUROC 0.111 for leakage — systematically worse than random guessing.