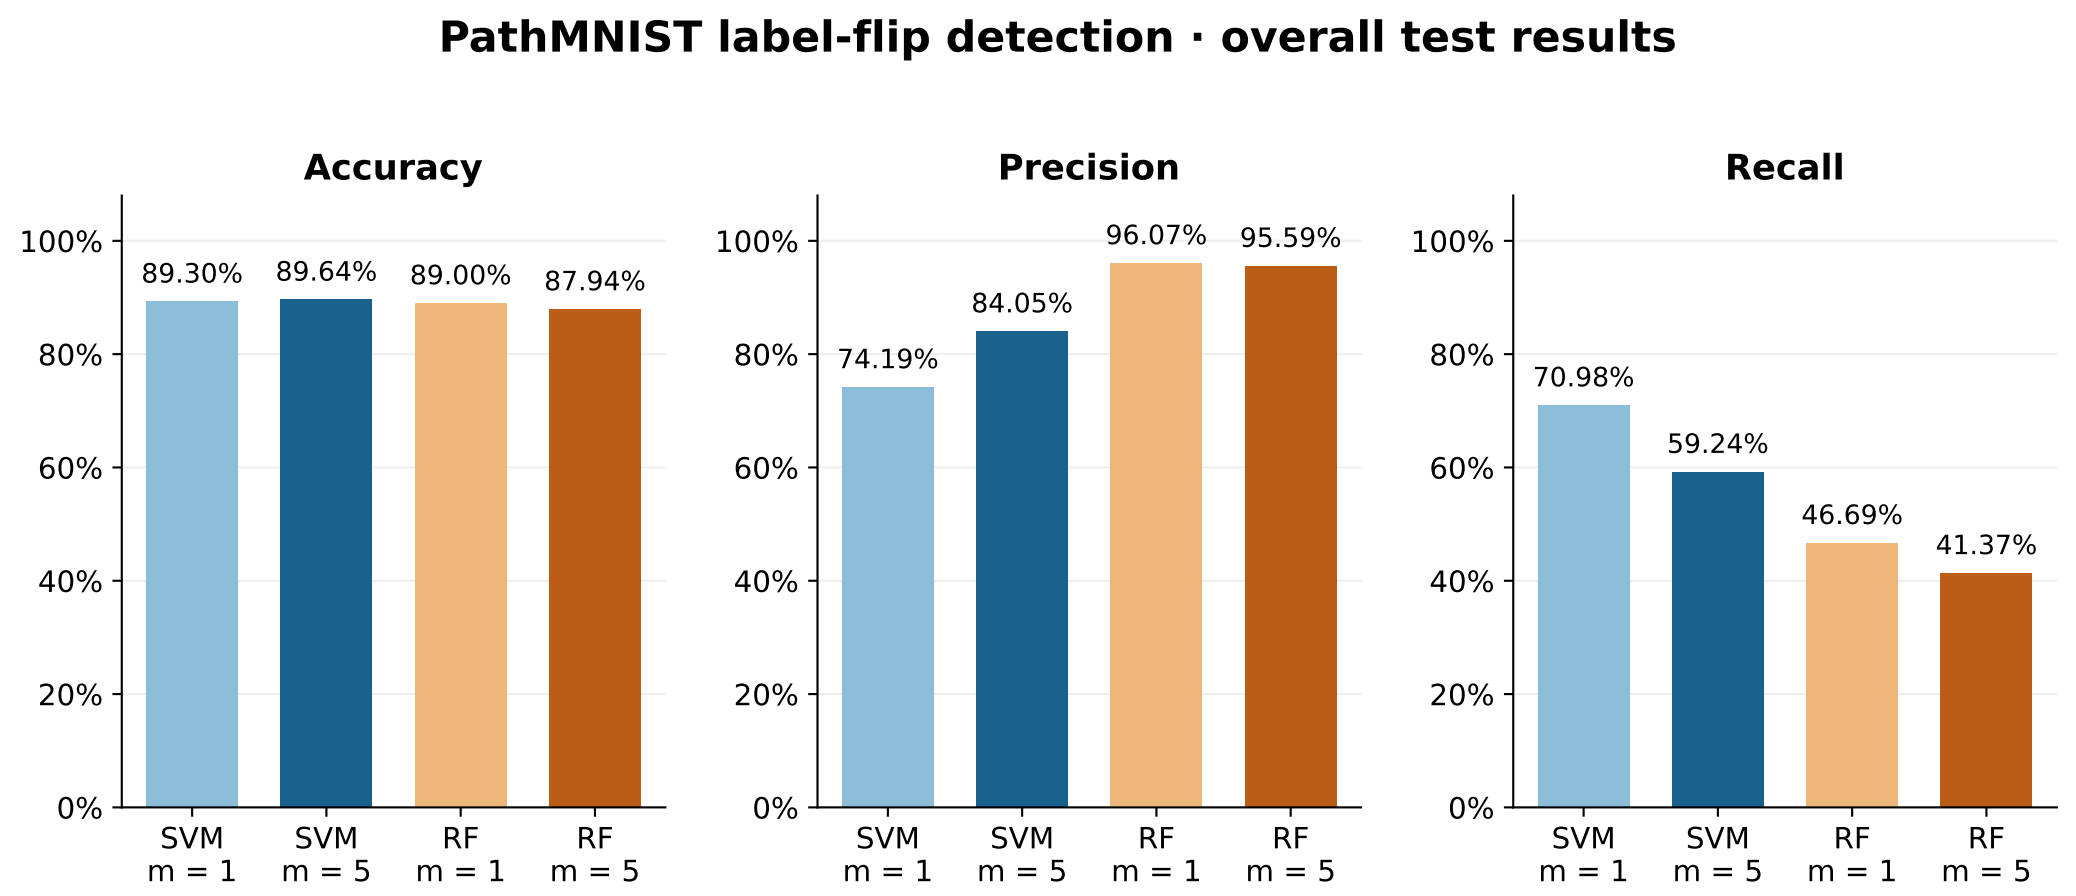
PathMNIST label-flip detection · overall test results
Accuracy
Precision
Recall
100%
80%
60%
40%
20%
0%
89.30%
89.64%
89.00%
87.94%
74.19%
84.05%
96.07%
95.59%
70.98%
59.24%
46.69%
41.37%
SVM m = 1
SVM m = 5
RF m = 1
RF m = 5
5,000 test samples · 996 poisoned · seed 42 · positive = poisoned / reject
Precision: how often a rejection is correct. Recall: how much poison is detected.