


# Referencing Schemes

# Options

1. External reference
2. Device reference

# External reference

- Connect a needle probes to **Ref1** or **Ref2**
- **Orange circles** indicate the **down position** of the switches
- The configuration makes it so that none of the depth electrodes are connected to reference

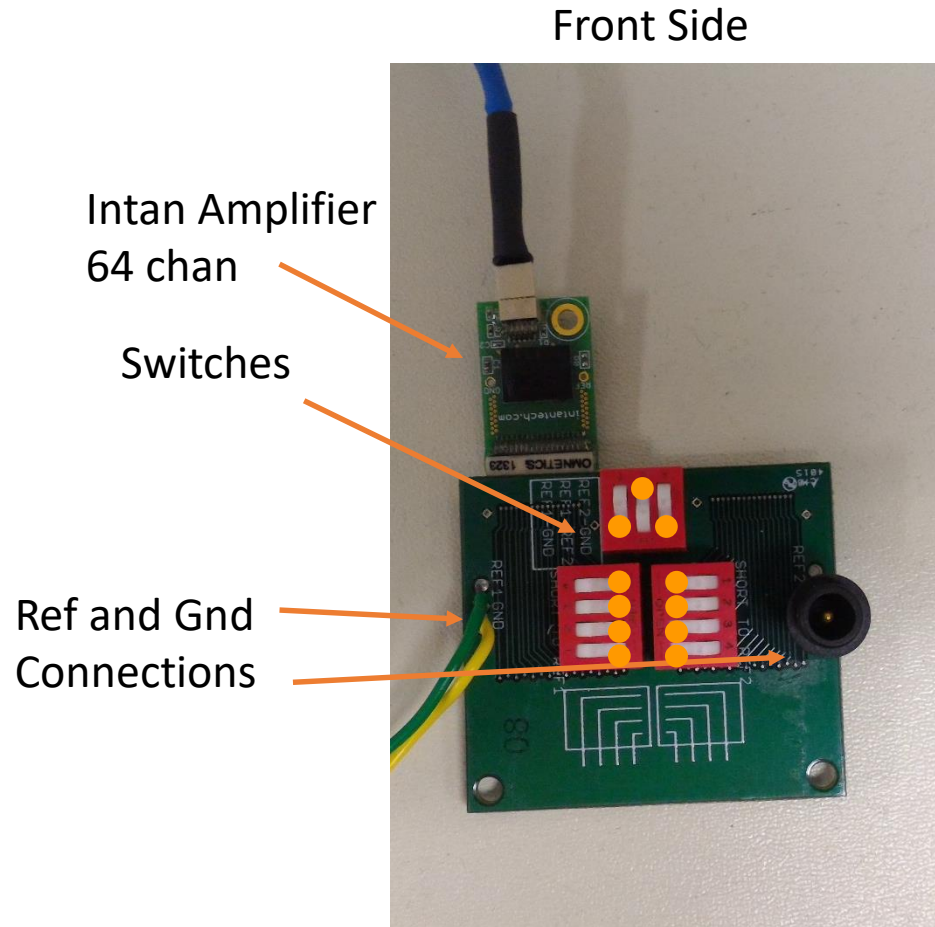

# Depth Channel Reference

- Ensure that the **macro electrode** are connected to the **inner ribbon channels** are indicated by the arrows
- Positions the switches are according to the orange dots

