


Thorax

Balanced Accuracy in sample

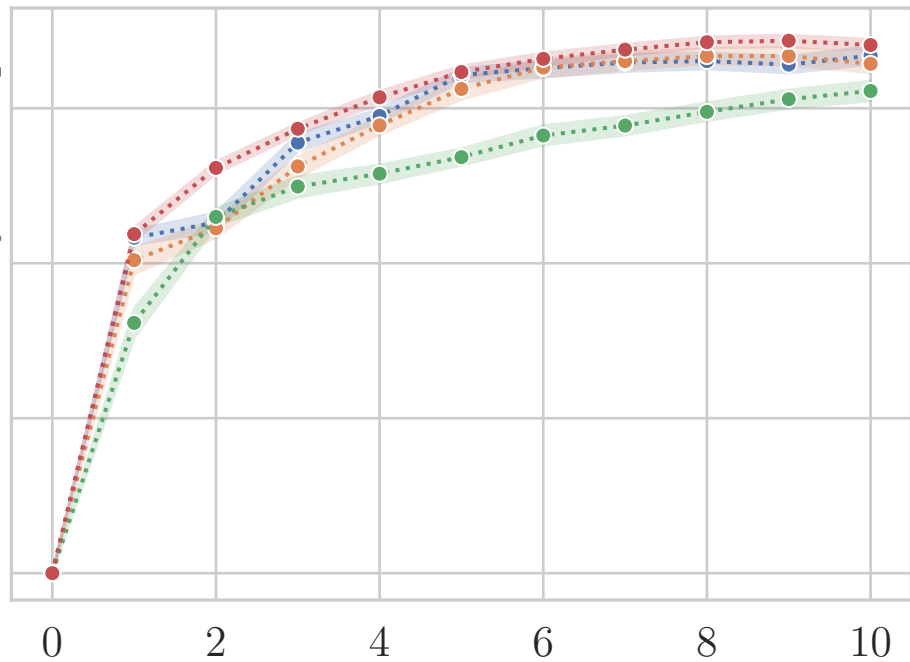

0.8

0.7

0.6

0.5

Expected Entropy Precision@0.9 Accuracy Balanced Accuracy

Balanced Accuracy out of sample

