


Thorax


Precision@0.9 in sample

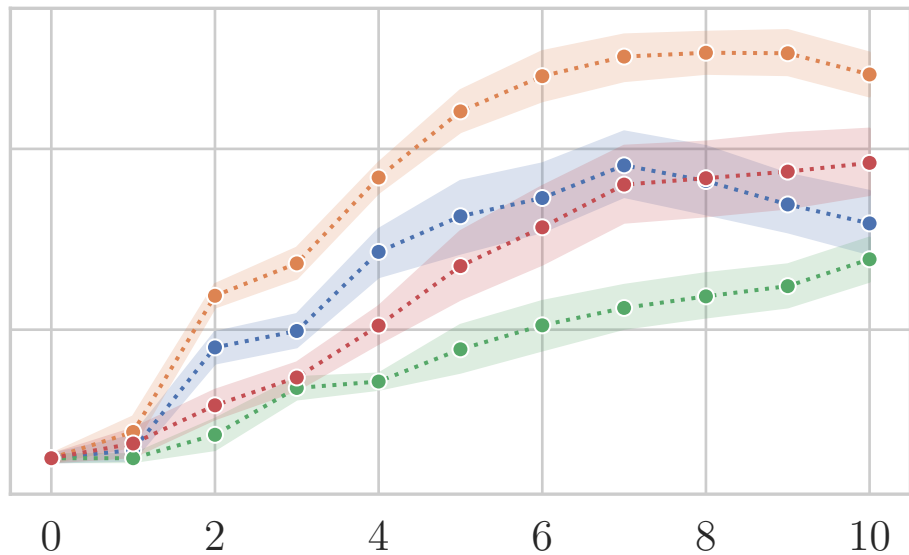

0.3


0.2

Precision@0.9 out of sample

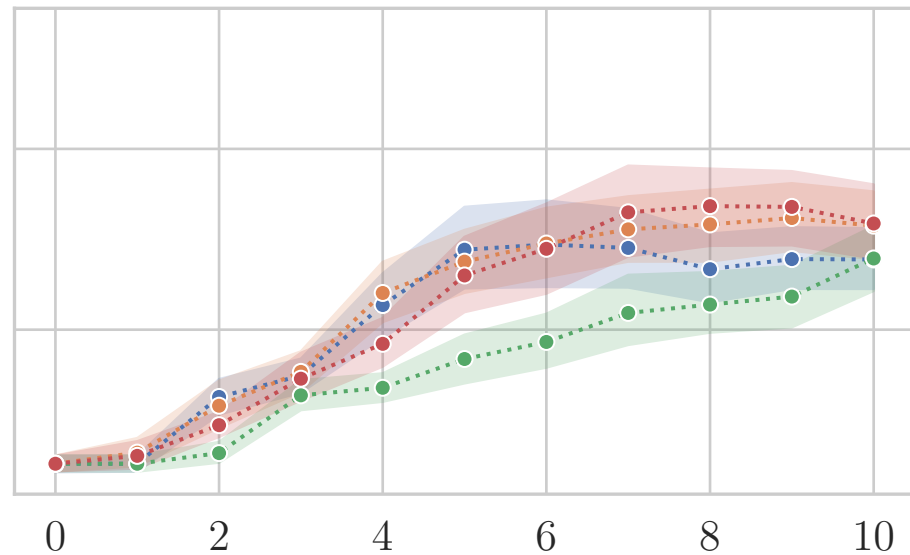

Breast

Precision@0.9 in sample

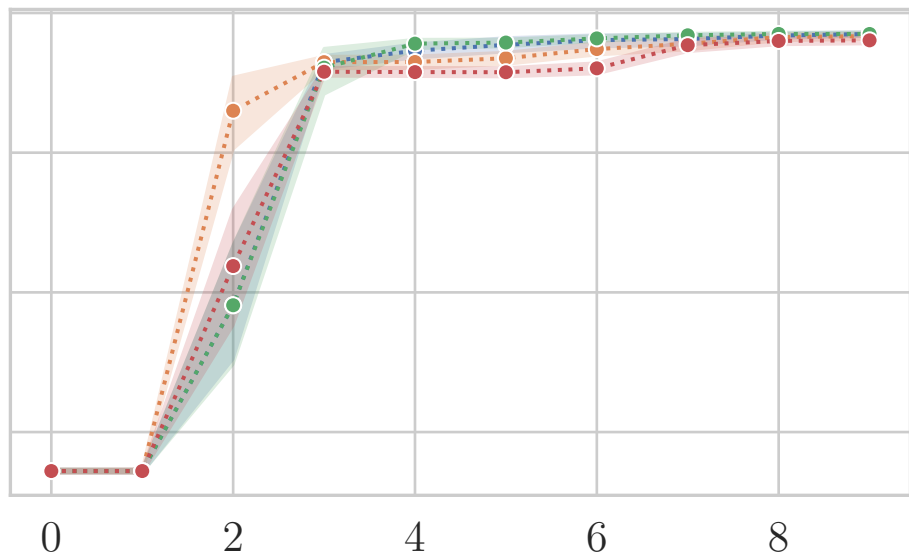


1.0

0.8

0.6

0.4

Precision@0.9 out of sample

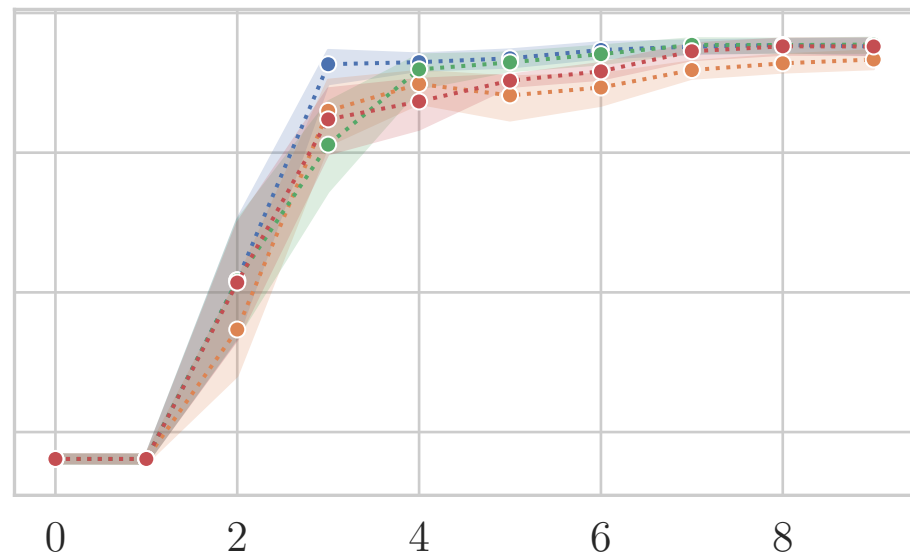

Expected Entropy Precision@0.9 Accuracy Balanced Accuracy