

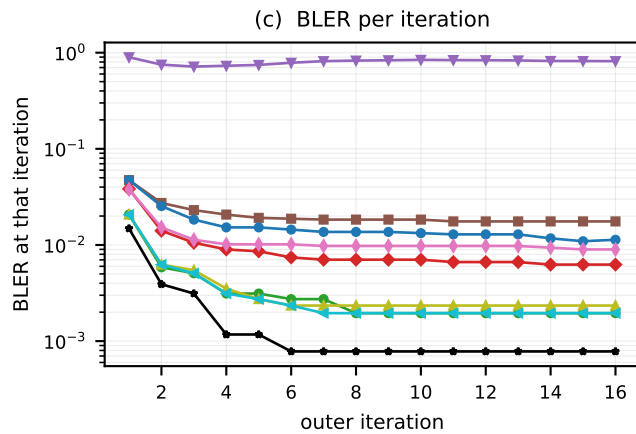


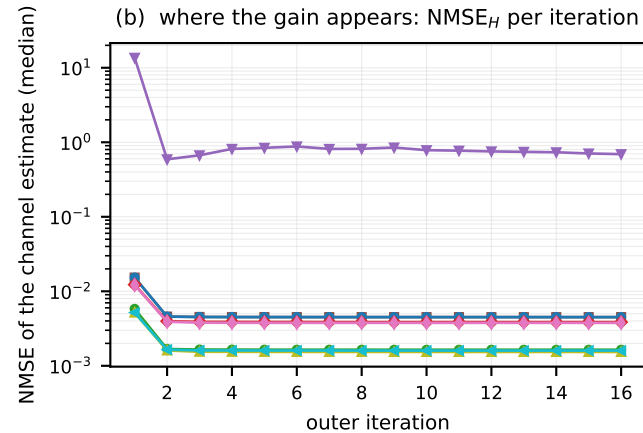

(d) cavity variance the denoiser is asked for [diagnostic not yet run]

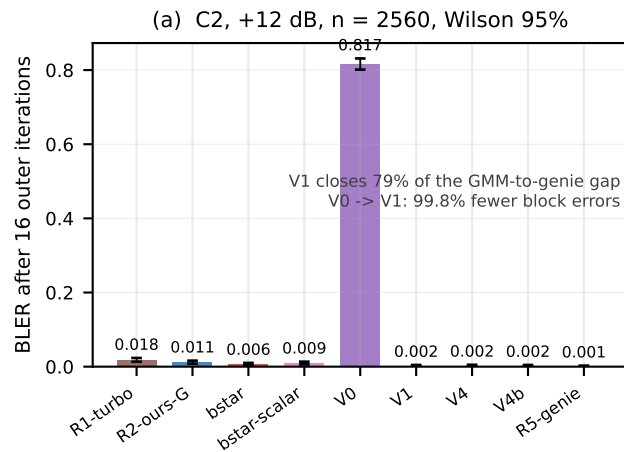