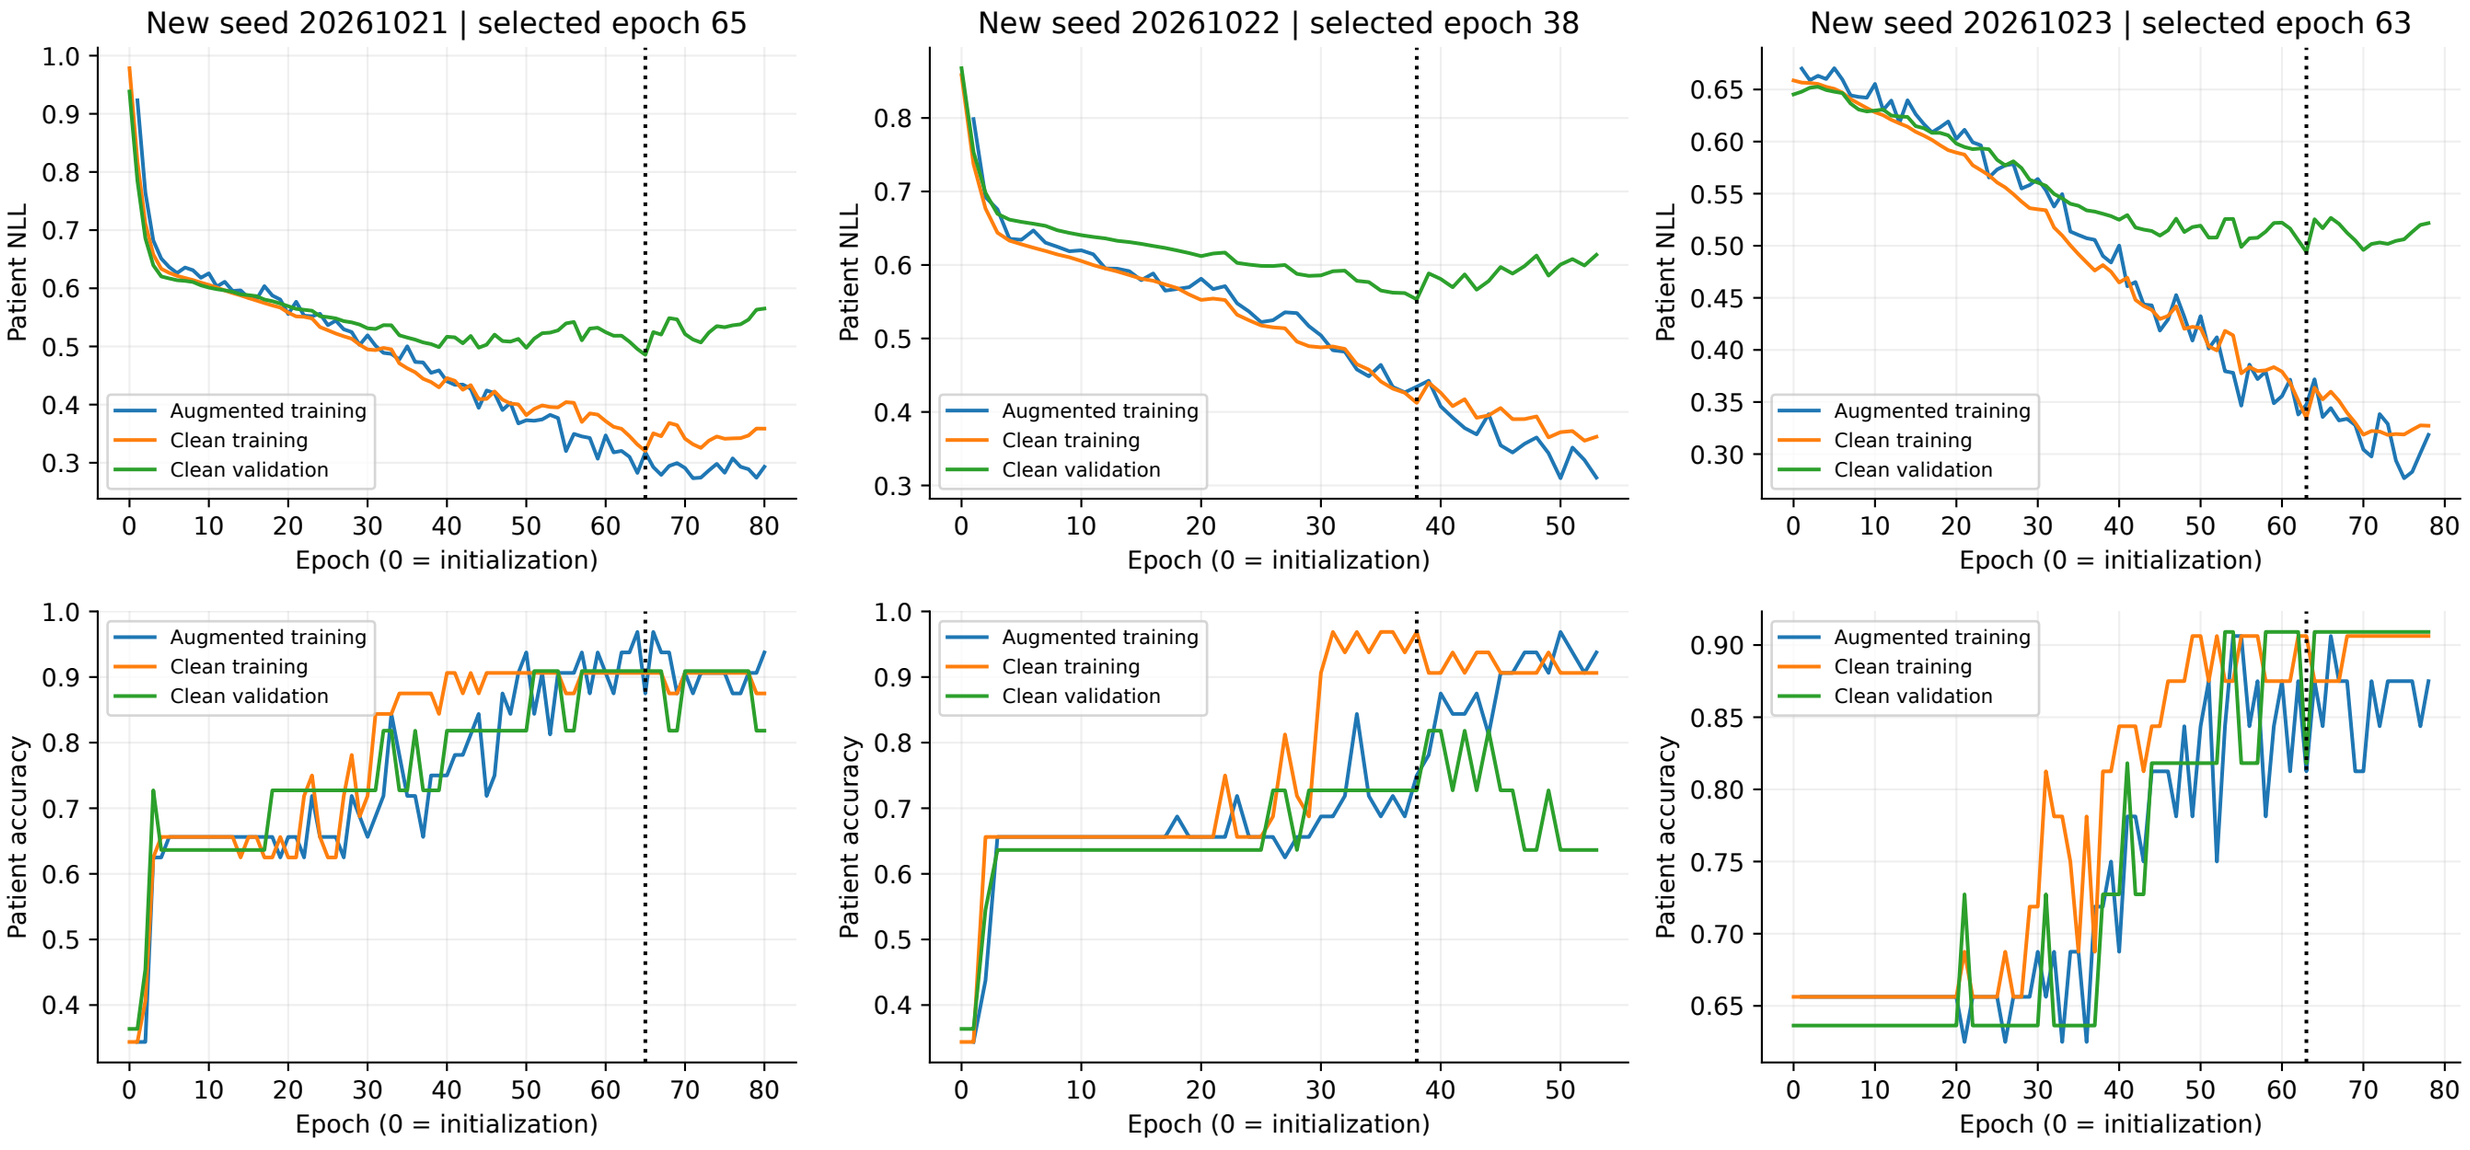


32 training and 11 validation patients. Clean training is resubstitution; augmentation is applied only to optimization draws.
Stored trainer NLL uses its fixed 1e-15 clipping; held-out NLL uses the frozen comparison helper 1e-12 clipping.