
$TP16 \quad Printed: Wednesday, October 05, 2022 \ 10:17:17 \\ C: Users \cup Documents \cup OmniSEC \ Data \ THF \ 2022-10-04 \ 2022-10-04 \ 21;32;38 \ TP16 \ 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	15.553
Mn - (Daltons)	20,375
Mw - (Daltons)	31,731
Mz - (Daltons)	45,542
Mp - (Daltons)	28,597
Mw / Mn	1.557
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	7,692
Mw 10.0% High	78,098
Wt Fr (Peak)	1.000
RI Area - (mvml)	180.10
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0003.vcm
Limits File	
Date Acquired	Oct 04, 2022 - 21:32:38
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

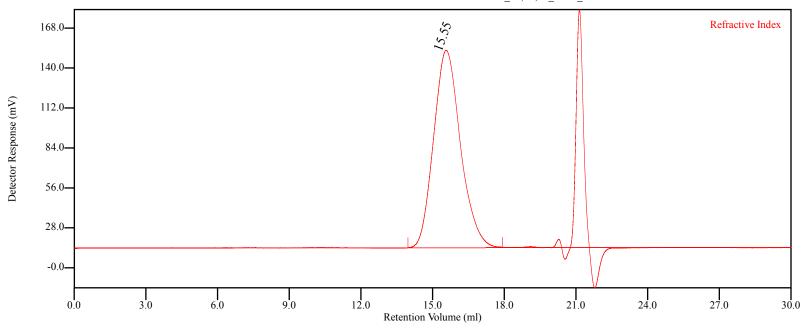