
$TP42 \quad Printed: Wednesday, December 07, 2022 \ 10:42:35 \\ C: \ Users \ VomniSEC \ Data \ THF \ 2022-12-06 \ 2022-12-06 \ 14;31;55 \ TP42 \ 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	16.617
Mn - (Daltons)	6,543
Mw - (Daltons)	10,328
Mz - (Daltons)	15,390
Mp - (Daltons)	8,360
Mw / Mn	1.578
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	2,556
Mw 10.0% High	26,586
Wt Fr (Peak)	1.000
RI Area - (mvml)	618.00
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Dec 06, 2022 - 14:31:55
Solvent	THF
Acquisition Operator	ADMIN : Administrator
Calculation Operator	ADMIN : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

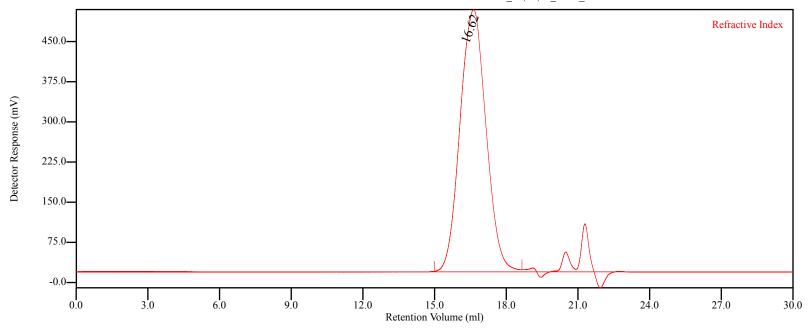