
$TP20 \ \ Printed: Wednesday, October 05, 2022 \ 10:18:24 \\ C:\Users\user\Documents\OmniSEC \ Data\THF\2022-10-04\2022-10-04_23;37;03_TP20_01.vdt$



Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	15.707
Mn - (Daltons)	17,836
Mw - (Daltons)	26,328
Mz - (Daltons)	36,768
Mp - (Daltons)	23,600
Mw / Mn	1.476
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	7,122
Mw 10.0% High	63,027
Wt Fr (Peak)	1.000
RI Area - (mvml)	308.87
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0003.vcm
Limits File	
Date Acquired	Oct 04, 2022 - 23:37:03
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

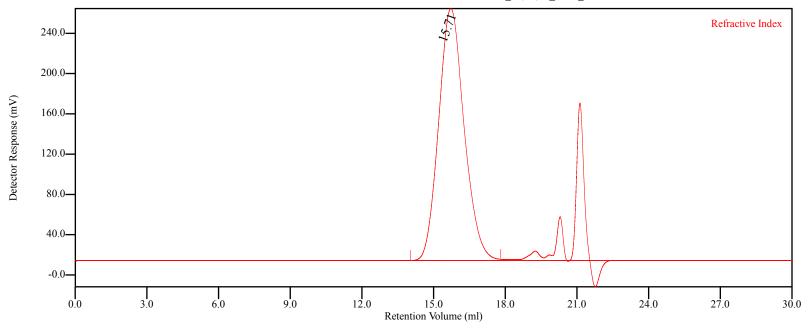