
TP75 Printed: Wednesday, March 01, 2023 14:29:30 C:\Users\user\Documents\OmniSEC Data\THF\2023-02-28\2023-02-28_20;08;40_TP75_01.vdt



Conventional	Calibration	Homopolymers	· Daculte

Peak RV - (ml)	16.137
Mn - (Daltons)	11,483
Mw - (Daltons)	16,873
Mz - (Daltons)	23,713
Mp - (Daltons)	15,118
Mw / Mn	1.469
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	4,628
Mw 10.0% High	40,676
Wt Fr (Peak)	1.000
RI Area - (mvml)	209.81
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 20:08:40
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

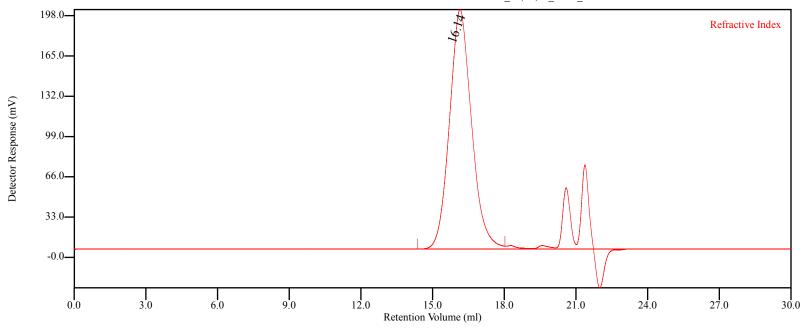