
$TP54\ \ Printed:\ Wednesday,\ January\ 18,\ 2023\ 14:56:54\\ C:\ Users\ \ VomniSEC\ Data\ THF\ 2023-01-17\ 2023-01-18\ 03;20;58\ TP54\ 01.vdt$



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	16.413
Mn - (Daltons)	7,080
Mw - (Daltons)	11,862
Mz - (Daltons)	18,040
Mp - (Daltons)	10,274
Mw / Mn	1.675
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	2,584
Mw 10.0% High	30,967
Wt Fr (Peak)	1.000
RI Area - (mvml)	215.27
UV Area - (mvml)	0.00

Annotation	
Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Jan 18, 2023 - 03:20:58
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

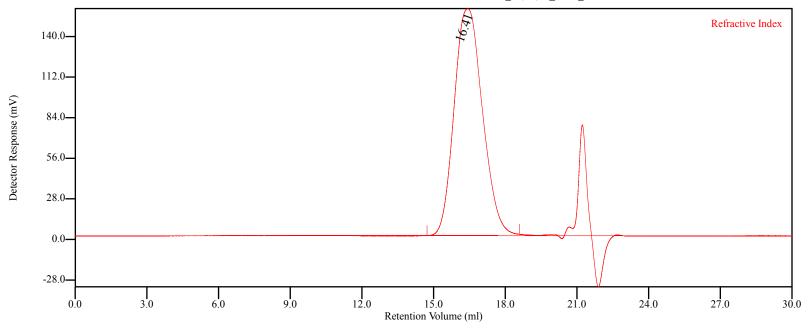