
$TP40 \quad Printed: Wednesday, December 07, 2022 \ 10:42:08 \\ C: \ Users \ VomniSEC \ Data \ THF \ 2022-12-06 \ 2022-12-06 \ 13;29;42 \ TP40 \ 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	16.223
Mn - (Daltons)	9,118
Mw - (Daltons)	15,157
Mz - (Daltons)	22,514
Mp - (Daltons)	14,160
Mw / Mn	1.662
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	3,366
Mw 10.0% High	38,703
Wt Fr (Peak)	1.000
RI Area - (mvml)	337.97
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Dec 06, 2022 - 13:29:42
Solvent	THF
Acquisition Operator	ADMIN : Administrator
Calculation Operator	ADMIN : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

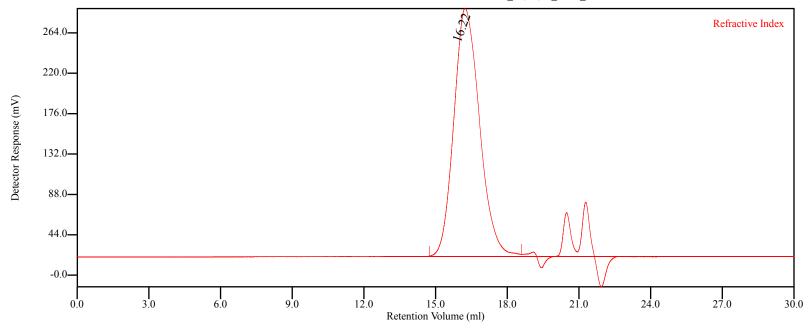