
## TP92 Printed: Friday, April 14, 2023 10:59:41 C:\Users\user\Documents\OmniSEC Data\THF\2023-04-13\2023-04-13\_22;18;18\_TP92\_01.vdt



## Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	16.063
Mn - (Daltons)	12,125
Mw - (Daltons)	18,436
Mz - (Daltons)	25,832
Mp - (Daltons)	17,205
Mw / Mn	1.520
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	4,600
Mw 10.0% High	43,969
Wt Fr (Peak)	1.000
RI Area - (mvml)	113.13
UV Area - (mvml)	0.00

Annotation	
M. d. 153	PG COMPANA
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Apr 13, 2023 - 22:18:18
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

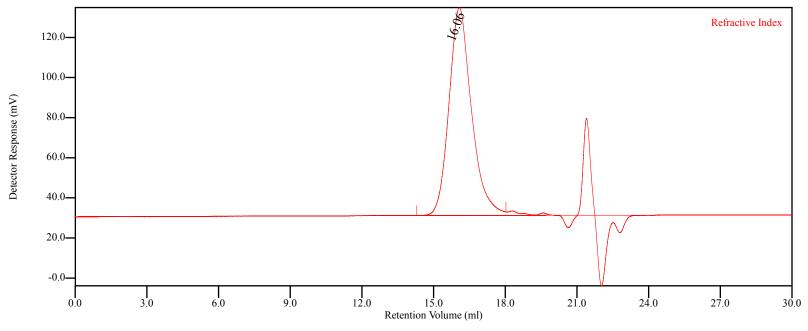