
$TP59 \quad Printed: Wednesday, January 18, 2023 \ 14:57:56 \\ C: Users \cup Documents \cup OmniSEC \ Data \setminus THF \setminus 2023-01-17 \setminus 2023-01-18 \ 05;56;28 \ TP59 \ 01.vdt$



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	15.580
Mn - (Daltons)	22,988
Mw - (Daltons)	36,332
Mz - (Daltons)	54,004
Mp - (Daltons)	31,583
Mw / Mn	1.580
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	8,803
Mw 10.0% High	92,703
Wt Fr (Peak)	1.000
RI Area - (mvml)	131.46
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Jan 18, 2023 - 05:56:28
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

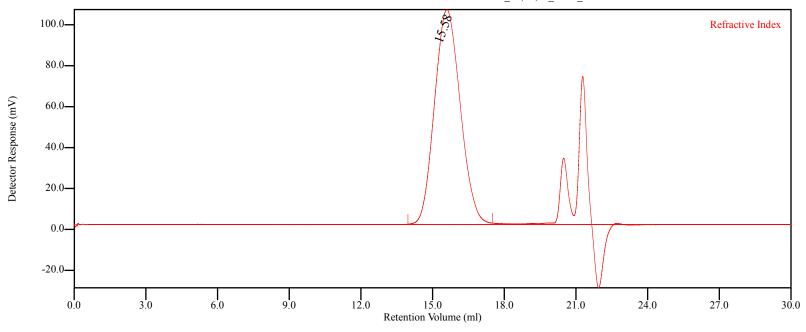