
TP72 Printed: Wednesday, March 01, 2023 14:28:47 C:\Users\user\Documents\OmniSEC Data\THF\2023-02-28\2023-02-28_18;35;22_TP72_01.vdt



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	15.603
Mn - (Daltons)	22,253
Mw - (Daltons)	36,518
Mz - (Daltons)	54,867
Mp - (Daltons)	31,033
Mw / Mn	1.641
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	8,360
Mw 10.0% High	94,657
Wt Fr (Peak)	1.000
RI Area - (mvml)	115.64
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 18:35:22
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

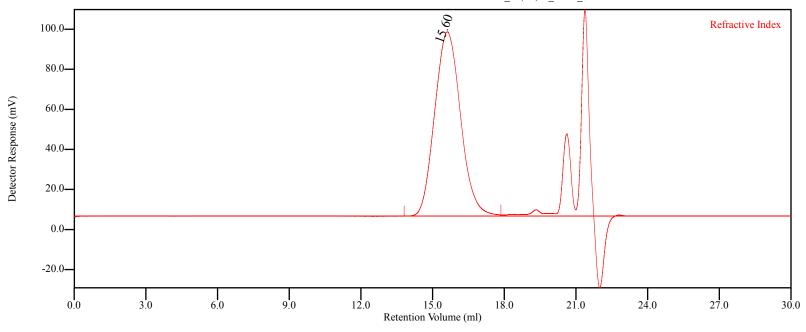