
$TP43 \quad Printed: Wednesday, December 07, 2022 \ 10:42:45 \\ C: \ Users \ VomniSEC \ Data \ THF \ 2022-12-06 \ 2022-12-06 \ 15;03;00 \ TP43 \ 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	15.443
Mn - (Daltons)	31,613
Mw - (Daltons)	61,729
Mz - (Daltons)	111,989
Mp - (Daltons)	40,567
Mw / Mn	1.953
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	11,169
Mw 10.0% High	191,622
Wt Fr (Peak)	1.000
RI Area - (mvml)	509.06
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcn
Limits File	
Date Acquired	Dec 06, 2022 - 15:03:00
Solvent	THI
Acquisition Operator	ADMIN : Administrator
Calculation Operator	ADMIN : Administrator
Column Set	2 x PLGel Mixed-F
System	THI
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	400

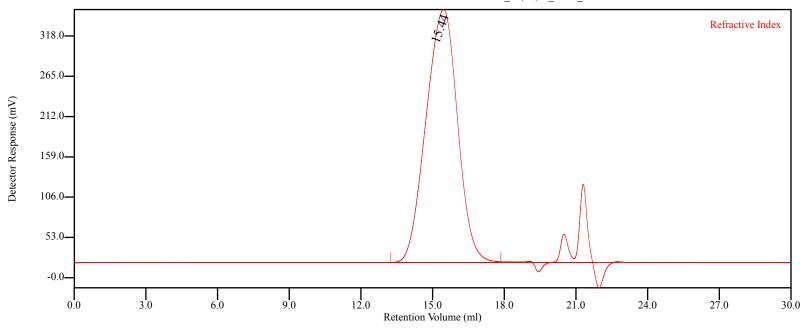