
$TP76 \ \ Printed: Wednesday, March 01, 2023 \ 14:29:42 \\ C:\Users\user\Documents\OmniSEC \ Data\THF\2023-02-28\2023-02-28\20;39;47_TP76_01.vdt$



Conventional	Colibration	 Homonolymers · Results 	

Peak RV - (ml)	15.913
Mn - (Daltons)	14,512
Mw - (Daltons)	23,473
Mz - (Daltons)	35,020
Mp - (Daltons)	20,350
Mw / Mn	1.617
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	5,406
Mw 10.0% High	60,460
Wt Fr (Peak)	1.000
RI Area - (mvml)	315.55
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 20:39:47
Solvent	THE
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THE
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

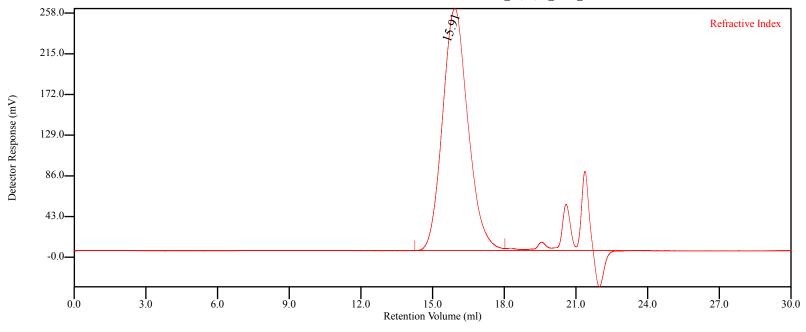