
TP79 Printed: Wednesday, March 01, 2023 14:30:25 C:\Users\user\Documents\OmniSEC Data\THF\2023-02-28\2023-02-28_22;13;05_TP79_01.vdt



Conventional Calibration - Homopolymers : Res	ults
---	------

Peak RV - (ml)	15.853
Mn - (Daltons)	15,391
Mw - (Daltons)	25,286
Mz - (Daltons)	38,211
Mp - (Daltons)	22,111
Mw / Mn	1.643
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	5,630
Mw 10.0% High	65,814
Wt Fr (Peak)	1.000
RI Area - (mvml)	161.82
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 22:13:05
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

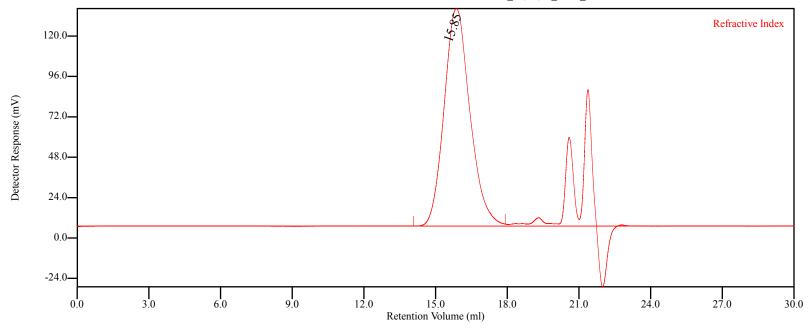