
$TP51 \quad Printed: Wednesday, January 18, 2023 \ 14:56:19 \\ C: Users \cup Documents \cup OmniSEC \ Data \setminus THF \setminus 2023-01-17 \setminus 2023-01-18 = 01;47;40 = TP51 = 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	15.///
Mn - (Daltons)	17,209
Mw - (Daltons)	27,387
Mz - (Daltons)	40,091
Mp - (Daltons)	24,153
Mw / Mn	1.591
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	6,438
Mw 10.0% High	68,977
Wt Fr (Peak)	1.000
RI Area - (mvml)	323.96
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Jan 18, 2023 - 01:47:40
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

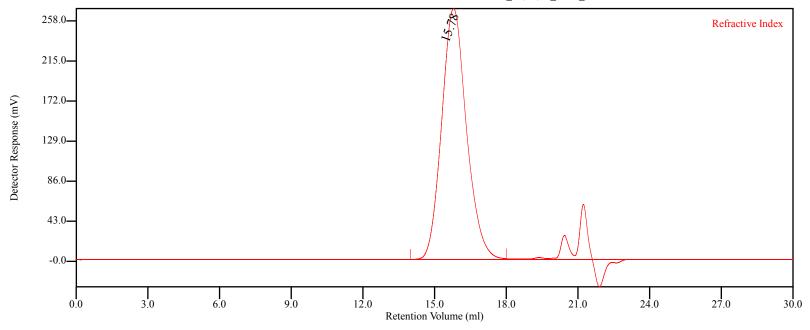