
TP7 Printed: Thursday, September 08, 2022 15:46:49 C:\Users\user\Documents\OmniSEC Data\THF\2022-09-07\2022-09-07_20;06;58_TP7_01.vdt



Conventional	Calibration -	Homopolymers	Reculte

Peak RV - (ml)	16.033
Mn - (Daltons)	13,005
Mw - (Daltons)	20,490
Mz - (Daltons)	30,448
Mp - (Daltons)	17,271
Mw / Mn	1.575
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	5,025
Mw 10.0% High	52,750
Wt Fr (Peak)	1.000
RI Area - (mvml)	397.50
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0000.vcm
Limits File	
Date Acquired	Sep 07, 2022 - 20:06:58
Solvent	THE
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THE
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

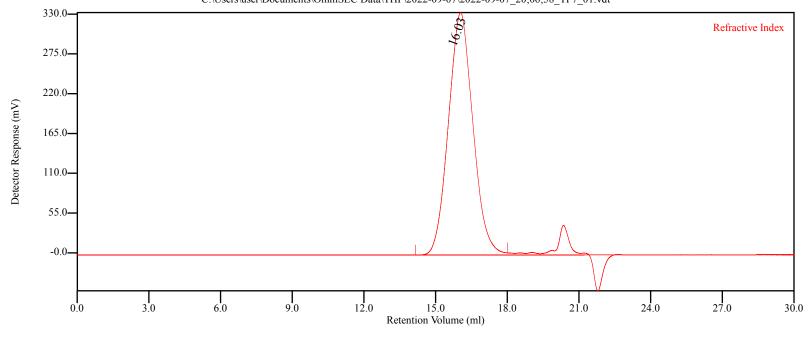