
$TP23 \quad Printed: Wednesday, October 05, 2022 \ 10:19:14 \\ C:\Users\user\Documents\OmniSEC \ Data\THF\2022-10-04\2022-10-05_01;10;20_TP23_01.vdt$



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	15.813
Mn - (Daltons)	16,377
Mw - (Daltons)	24,354
Mz - (Daltons)	34,597
Mp - (Daltons)	20,723
Mw / Mn	1.487
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	6,612
Mw 10.0% High	59,628
Wt Fr (Peak)	1.000
RI Area - (mvml)	475.84
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0003.vcm
Limits File	
Date Acquired	Oct 05, 2022 - 01:10:20
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

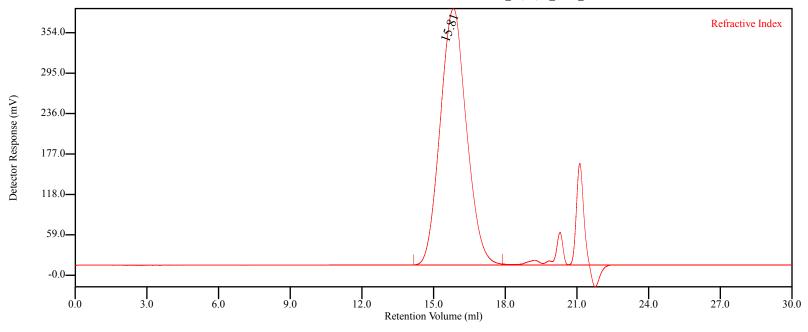