
$TP30 \ \ Printed: Friday, October 21, 2022 \ 09:39:39 \\ C: \ Users \ \ Documents \ OmniSEC \ Data \ THF \ 2022-10-20 \ 2022-10-20 \ 21;05;04_TP30_01.vdt$



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	15.853
Mn - (Daltons)	16,184
Mw - (Daltons)	21,566
Mz - (Daltons)	27,800
Mp - (Daltons)	19,723
Mw / Mn	1.333
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	7,156
Mw 10.0% High	46,799
Wt Fr (Peak)	1.000
RI Area - (mvml)	28.51
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0000.vcm
Limits File	ps conv occonven
Date Acquired	Oct 20, 2022 - 21:05:04
Solvent	THI
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-F
System	THI
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

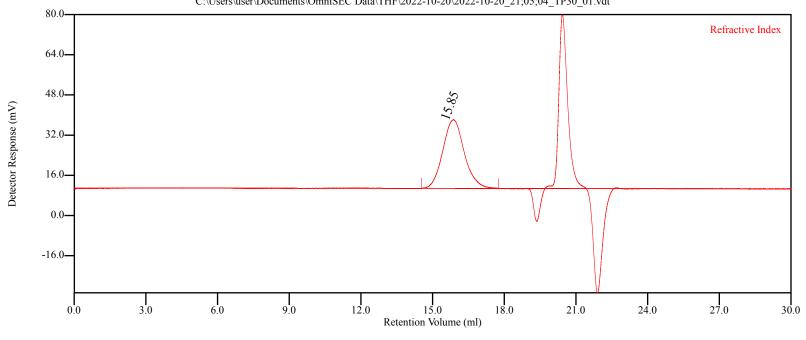