
$TP67 \ \ Printed: Wednesday, March 01, 2023 \ 14:27:40 \\ C:\ Users \ \ Documents \ OmniSEC \ Data \ THF \ 2023-02-28 \ 2023-02-28 \ 15;59;51 \ TP67 \ 01.vdt$



Conventional	Calibration .	Homonolymers · Results	

Peak RV - (ml)	15.677
Mn - (Daltons)	17,109
Mw - (Daltons)	31,459
Mz - (Daltons)	49,576
Mp - (Daltons)	28,157
Mw / Mn	1.839
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	5,689
Mw 10.0% High	85,282
Wt Fr (Peak)	1.000
RI Area - (mvml)	163.96
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 15:59:51
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

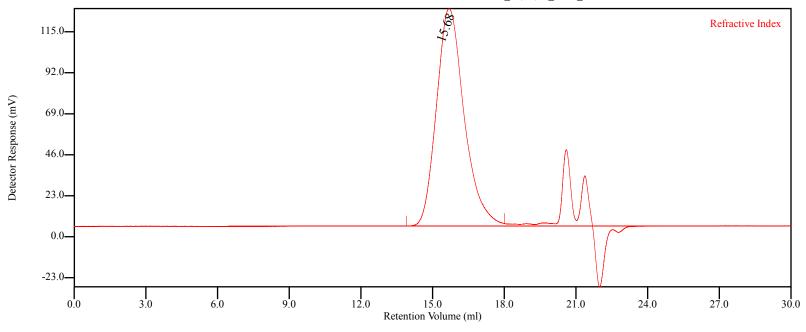