
$TP50 \quad Printed: Wednesday, January 18, 2023 \ 14:56:08 \\ C: Users \cup Documents \cup OmniSEC \ Data \setminus THF \setminus 2023-01-17 \setminus 2023-01-18 = 01;16;35 = TP50 = 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	16.577
Mn - (Daltons)	6,506
Mw - (Daltons)	10,170
Mz - (Daltons)	15,228
Mp - (Daltons)	8,244
Mw / Mn	1.563
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	2,560
Mw 10.0% High	26,276
Wt Fr (Peak)	1.000
RI Area - (mvml)	802.43
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Jan 18, 2023 - 01:16:35
Solvent	THI
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-E
System	THI
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

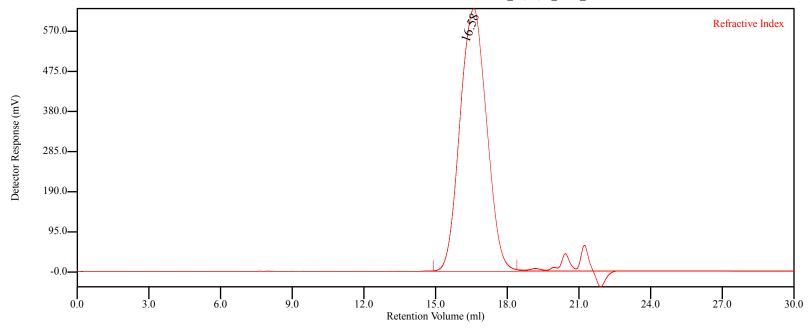