
## TP87 Printed: Friday, April 14, 2023 10:58:49 C:\Users\user\Documents\OmniSEC Data\THF\2023-04-13\2023-04-13\_19;42;47\_TP87\_01.vdt



## Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	15.680
Mn - (Daltons)	17,987
Mw - (Daltons)	31,303
Mz - (Daltons)	47,146
Mp - (Daltons)	28,784
Mw / Mn	1.740
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	6,230
Mw 10.0% High	80,645
Wt Fr (Peak)	1.000
RI Area - (mvml)	165.68
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Apr 13, 2023 - 19:42:47
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

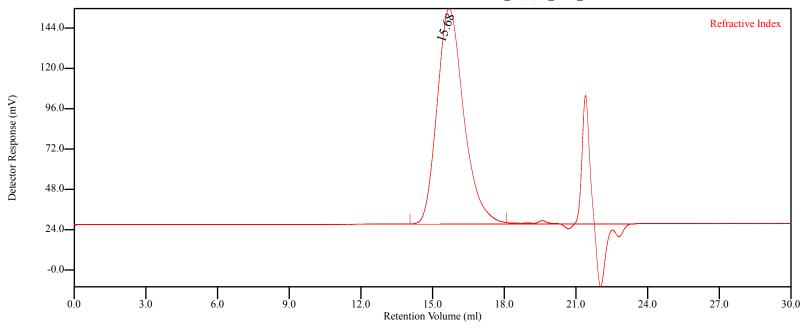