
TP73 Printed: Wednesday, March 01, 2023 14:28:58 C:\Users\user\Documents\OmniSEC Data\THF\2023-02-28\2023-02-28_19;06;28_TP73_01.vdt



Conventional Calibration - Homopolymers : Results

Peak RV - (ml)	15.883
Mn - (Daltons)	14,627
Mw - (Daltons)	23,966
Mz - (Daltons)	35,879
Mp - (Daltons)	21,274
Mw / Mn	1.639
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	5,340
Mw 10.0% High	61,669
Wt Fr (Peak)	1.000
RI Area - (mvml)	246.24
UV Area - (mvml)	0.00

Annotation	
Method File	PS CONV-0003.vcm
Limits File	
Date Acquired	Feb 28, 2023 - 19:06:28
Solvent	THE
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THE
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

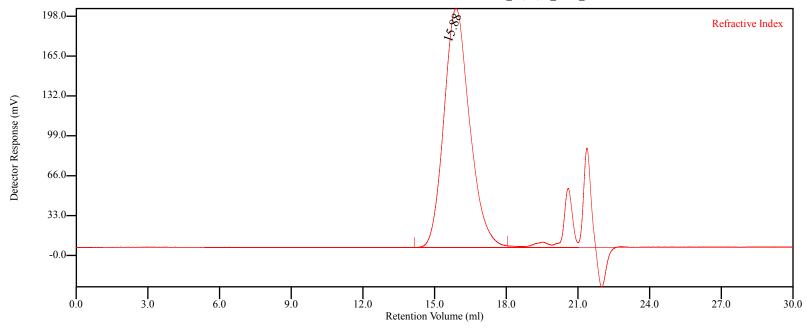