
$TP60\ \ Printed:\ Wednesday,\ January\ 18,\ 2023\ 14:58:11\\ C:\ Users\ \ Documents\ OmniSEC\ Data\ THF\ 2023-01-17\ 2023-01-18\ 06;27;35\ TP60\ 01.vdt$



Conventional	Calibration -	Homonolymers :	Regults

Peak RV - (ml)	15.423
Mn - (Daltons)	27,903
Mw - (Daltons)	44,869
Mz - (Daltons)	66,321
Mp - (Daltons)	39,054
Mw / Mn	1.608
Percent Above Mw: 0	100.000
Percent Below Mw: 0	0.000
Mw 10.0% Low	10,434
Mw 10.0% High	113,623
Wt Fr (Peak)	1.000
RI Area - (mvml)	77.75
UV Area - (mvml)	0.00

Annotation	
Method File	ps conv-0004.vcm
Limits File	
Date Acquired	Jan 18, 2023 - 06:27:35
Solvent	THF
Acquisition Operator	admin : Administrator
Calculation Operator	admin : Administrator
Column Set	2 x PLGel Mixed-B
System	THF
Flow Rate - (ml/min)	1.000
Inj Volume - (ul)	100.0
Volume Increment - (ml)	0.00333
Detector Temp (deg C)	40.0
Column Temp (deg C)	40.0
OmniSEC Build Number	406

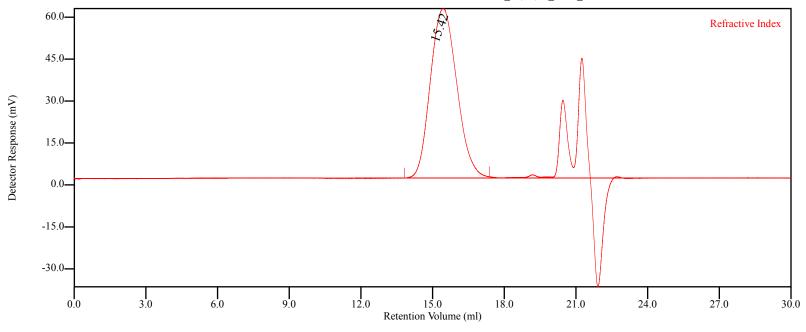