Biomedical Waste Classifier


Test-set model evaluation report

Metric	Result
Test samples	709
Test loss	0.0463
Top-1 accuracy	99.58%
Top-2 accuracy	100.00%
Macro precision	99.39%
Macro recall	99.54%
Macro F1 score	99.46%
Macro specificity	99.87%


Per-class metrics

Class	Precision	Recall	F1	Specificity	Support
Yellow	100.00%	100.00%	100.00%	100.00%	205
Red	100.00%	100.00%	100.00%	100.00%	220
Blue	97.56%	100.00%	98.77%	99.49%	120
White	100.00%	98.17%	99.08%	100.00%	164


Confusion matrix

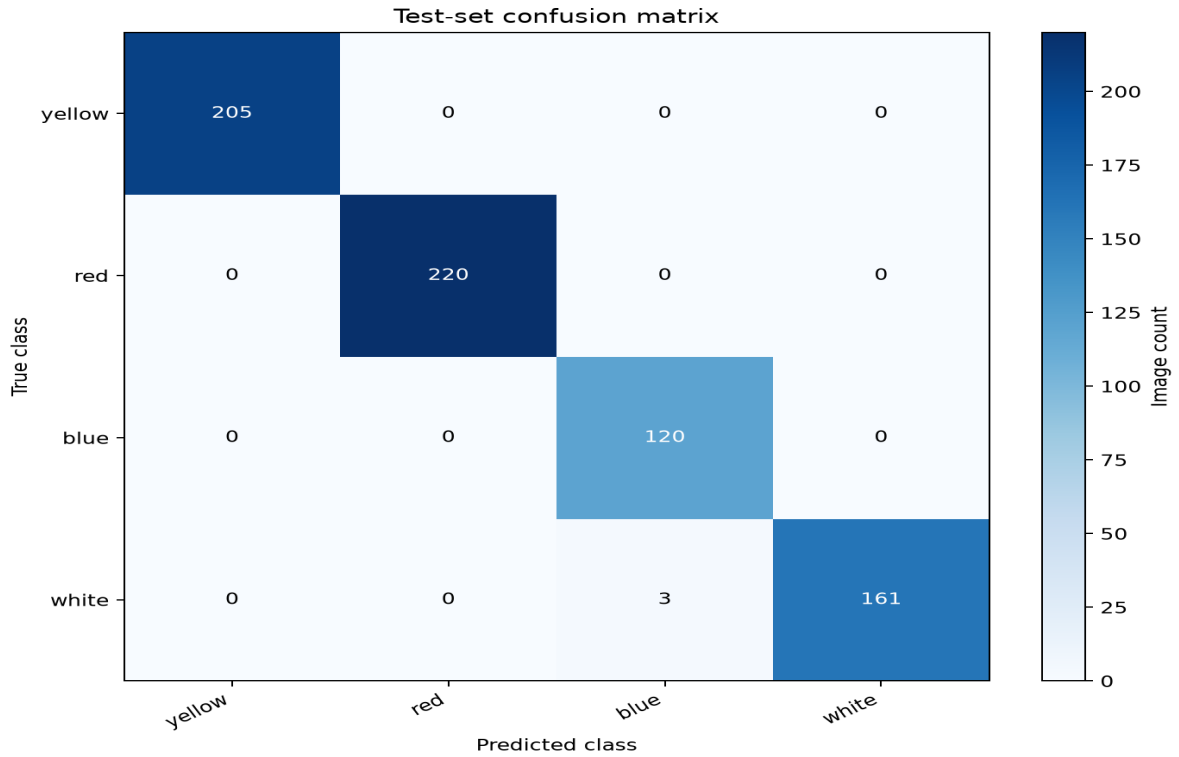


Per-class accuracy

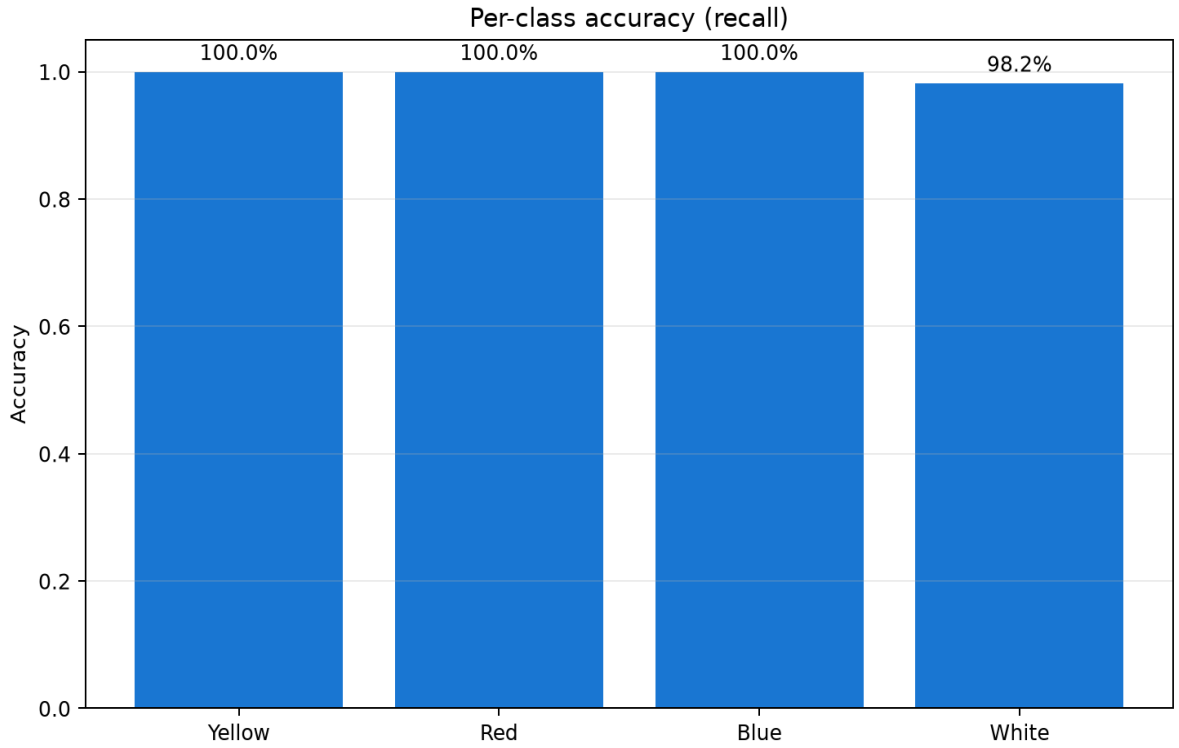


ROC curves

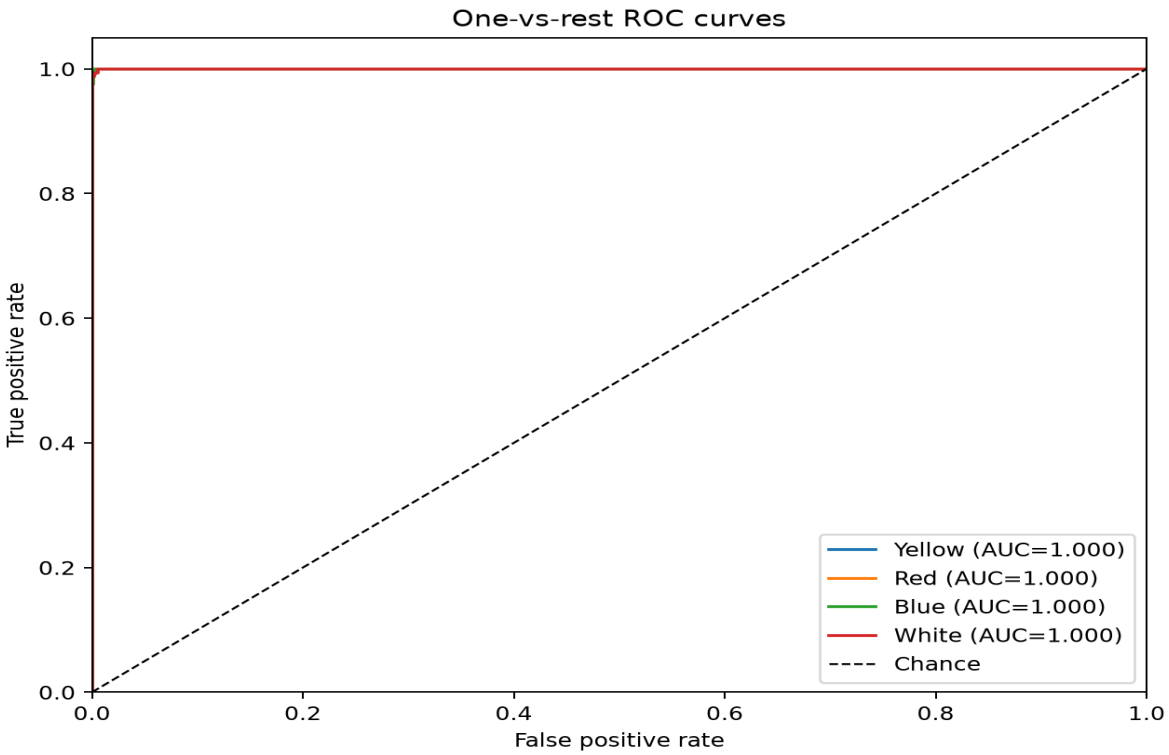

Precision-recall curves

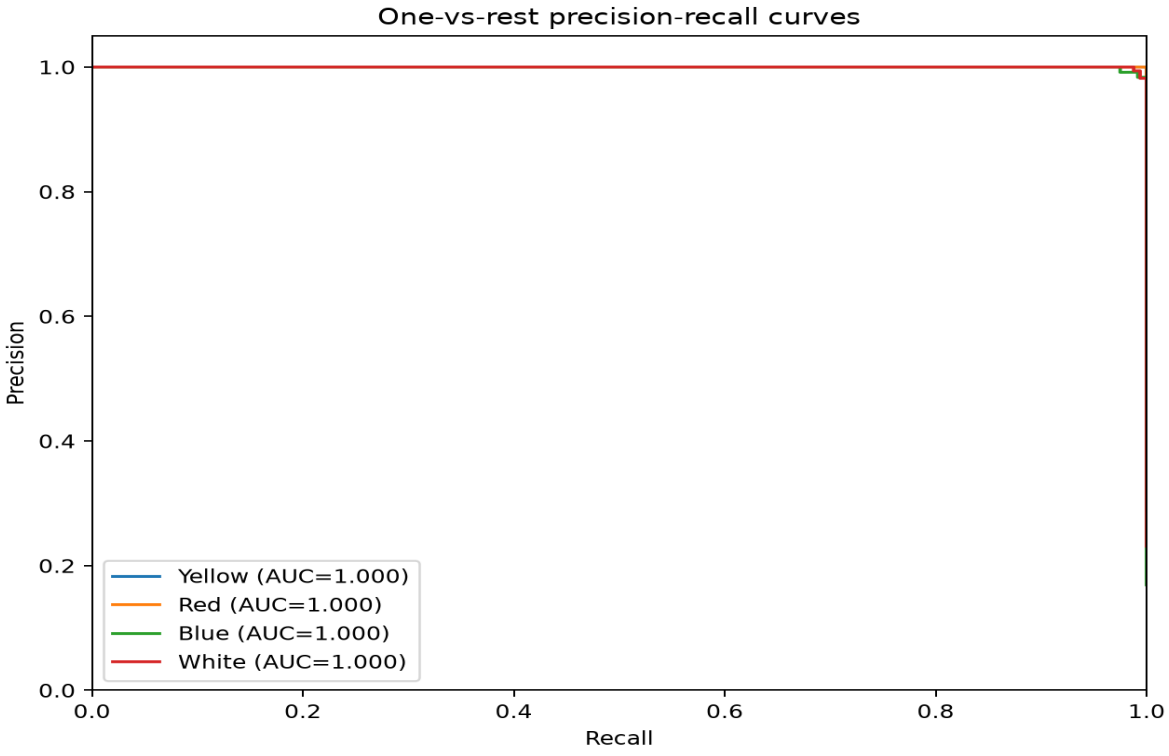

Prediction distribution

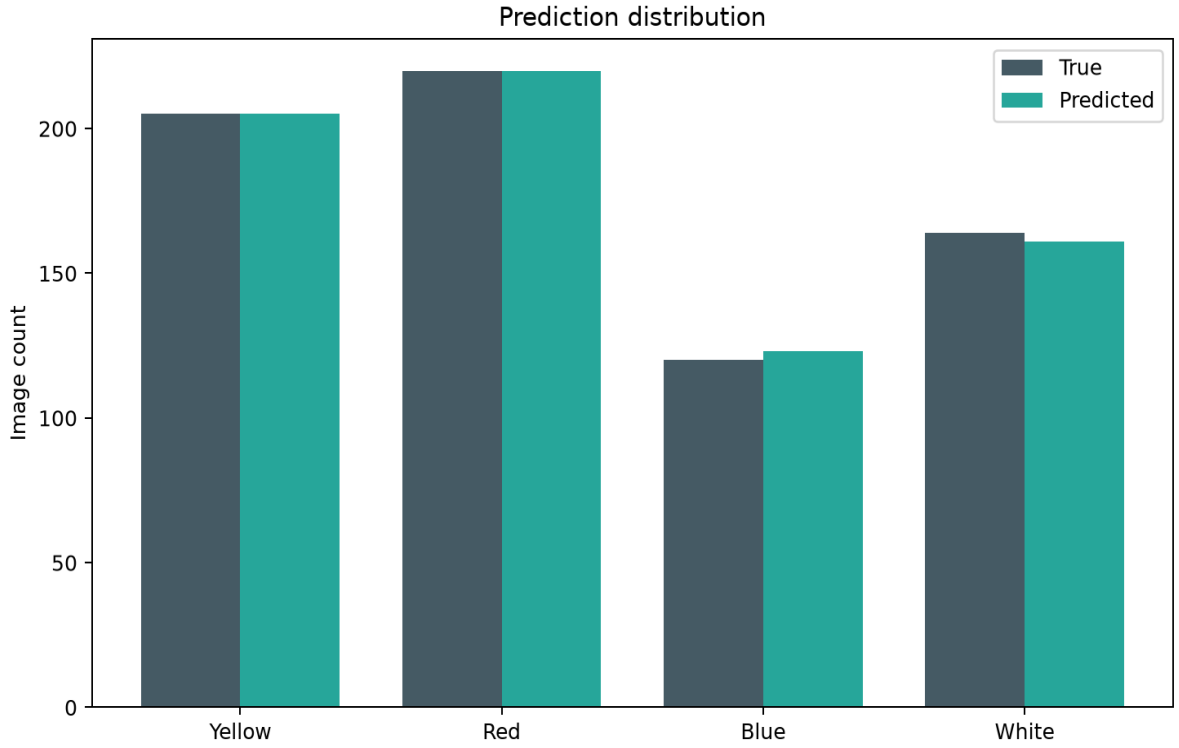
Prediction distribution
True
Predicted
Image count
0
50
100
150
200
Yellow
Red
Blue
White