



US0D1089658S

(12) **United States Design Patent** (10) **Patent No.:** **US D1,089,658 S**
Giphart et al. (45) **Date of Patent:** **** Aug. 19, 2025**

(54) **OCULAR DEVICE**

(71) Applicant: **ArcScan, Inc.**, Golden, CO (US)

(72) Inventors: **Johan Erik Giphart**, Aurora, CO (US);
Keir Hart, Lafayette, CO (US); **Barry
Schafer**, Folsom, CA (US); **Andrew K.
Levien**, Morrison, CO (US)

(73) Assignee: **ArcScan, Inc.**, Golden, CO (US)

(**) Term: **15 Years**

(21) Appl. No.: **29/824,355**

(22) Filed: **Jan. 24, 2022**

(51) **LOC (15) Cl.** **24-02**

(52) **U.S. Cl.**
USPC **D24/172**

(58) **Field of Classification Search**

USPC D24/170, 172, 185–187, 231, 232, 140,
D24/158–160, 120, 184, 137; D15/199;
D16/100, 130, 136, 200, 300
CPC A61B 3/02; A61B 3/0025; A61B 3/32;
A61B 3/024; A61B 3/028; A61B 3/12;
A61B 3/103; A61B 3/005; A61B 3/06;
A61B 3/0008; A61B 3/063; A61B 3/113;
A61B 3/0041; A61B 3/0091; A61B
5/7275; G06T 2207/30041; G02C 13/003;
G02C 3/003

See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

5,838,424 A * 11/1998 Wawro A61B 3/02
351/200
6,491,637 B2 12/2002 Foster et al.
6,887,203 B2 5/2005 Phillips et al.
D552,736 S * 10/2007 Yamaoka D24/172
D614,774 S * 4/2010 Gausmann D24/160

(Continued)

OTHER PUBLICATIONS

Why Using Arcscan Sets Apart Evo ICL Procedures. Oct. 28, 2022.
Site visited Mar. 15, 2024. [https://www.iqlaservision.com/blog/
why-using-arcscan-sets-apart-evo-icl-procedures/] (Year: 2022).*

(Continued)

Primary Examiner — Wendy L Arminio

Assistant Examiner — Maheen Khurshid

(74) *Attorney, Agent, or Firm* — Sheridan Ross P.C.

(57) **CLAIM**

The ornamental design for an ocular device as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an ocular device of the claimed design;

FIG. 2 is a front perspective view of the ocular device of FIG. 1;

FIG. 3 is a back perspective view of the ocular device of FIG. 1;

FIG. 4 is a front elevation view of the ocular device of FIG. 1;

FIG. 5 is a back elevation view of the ocular device of FIG. 1;



FIG. 6 is a right elevation view of the ocular device of FIG. 1;

FIG. 7 is a left elevation view of the ocular device of FIG. 1;

FIG. 8 is a top plan view of the ocular device of FIG. 1; and, FIG. 9 is a bottom plan view of the ocular device of FIG. 1.

The broken lines in the figures depict portions of the ocular device that form no part of the claimed design. In FIG. 1, the additional broken lines illustrating a table and monitor depict environmental structure and form no part of the claimed design.

1 Claim, 9 Drawing Sheets

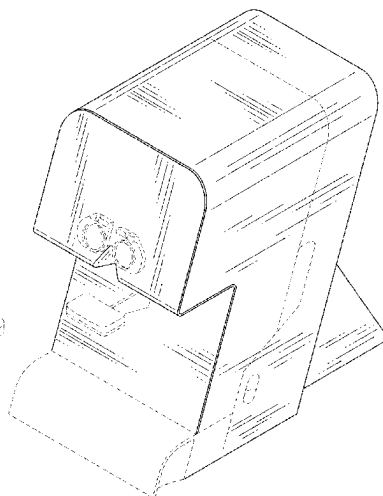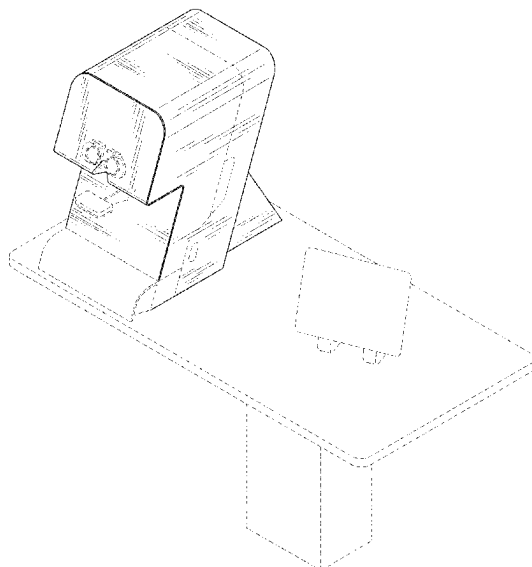

(56)

References Cited

U.S. PATENT DOCUMENTS

D638,128 S * 5/2011 Prokop D24/172
 8,317,709 B2 11/2012 Eilers et al.
 8,496,588 B2 7/2013 Eilers et al.
 8,510,883 B2 8/2013 Eilers et al.
 D698,444 S * 1/2014 Mensink D24/172
 D705,430 S * 5/2014 Sekine D24/172
 8,732,878 B2 5/2014 Eilers et al.
 8,758,252 B2 6/2014 Eilers et al.
 9,039,623 B2 5/2015 Eilers et al.
 D738,509 S * 9/2015 van Elzakker D24/172
 9,149,254 B2 10/2015 Watson
 9,320,427 B2 4/2016 Levien et al.
 D775,356 S * 12/2016 Zhou D24/172
 9,597,059 B2 3/2017 Watson et al.
 D816,218 S * 4/2018 Kambe D24/137
 10,265,049 B2 4/2019 Levien et al.
 D861,167 S * 9/2019 Emery D24/158

10,485,509 B2 11/2019 Eilers et al.
 10,531,859 B2 1/2020 Watson et al.
 10,736,605 B2 8/2020 Heath et al.
 10,888,301 B2 1/2021 Levien et al.
 11,357,479 B2 6/2022 Johnson
 2013/0237826 A1 9/2013 Levien
 2019/0290939 A1 9/2019 Watson et al.
 2021/0186458 A1 6/2021 Giphart et al.
 2021/0204906 A1 7/2021 Giphart et al.
 2021/0353252 A1 11/2021 Johnson et al.
 2021/0401401 A1 12/2021 Giphart et al.
 2022/0061801 A1 3/2022 Giphart et al.

OTHER PUBLICATIONS

Reichert Ocular Response Analyzer Measures Corneal Hysteresis (CH). Mar. 2, 2020. Site visited Mar. 15, 2024. [<https://www.youtube.com/watch?v=Y8-JKOg7QgU>] (Year: 2020).*

* cited by examiner

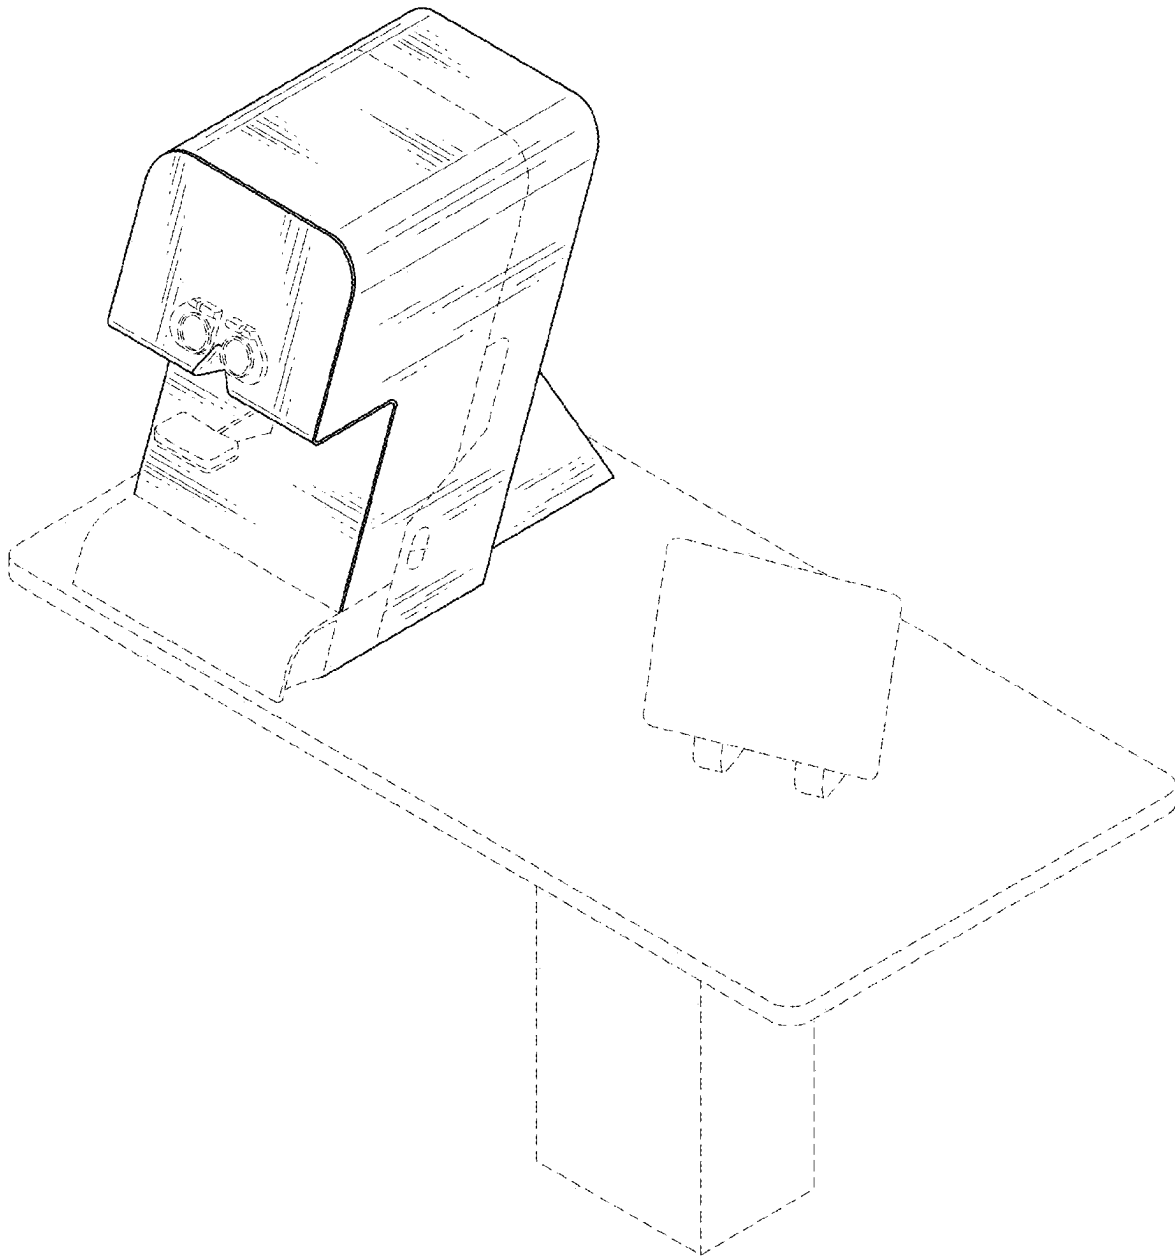


FIG.1

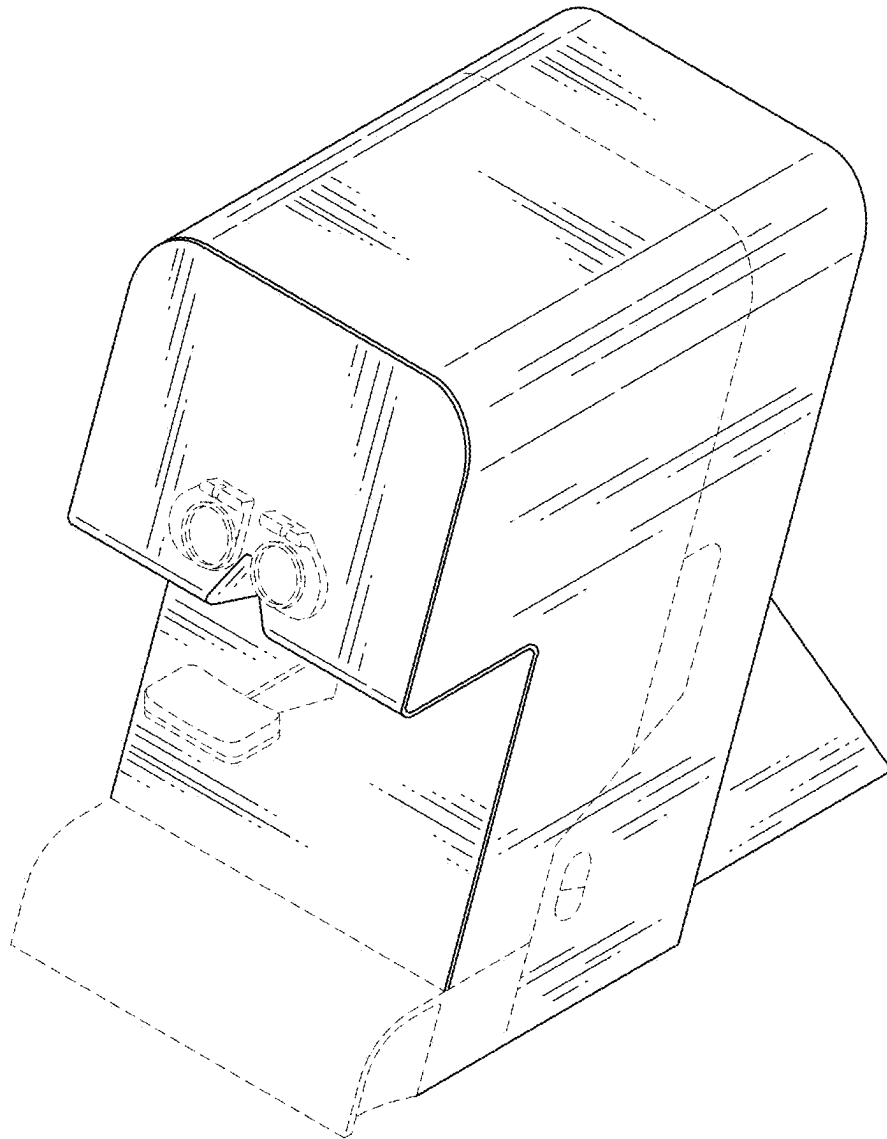


FIG.2

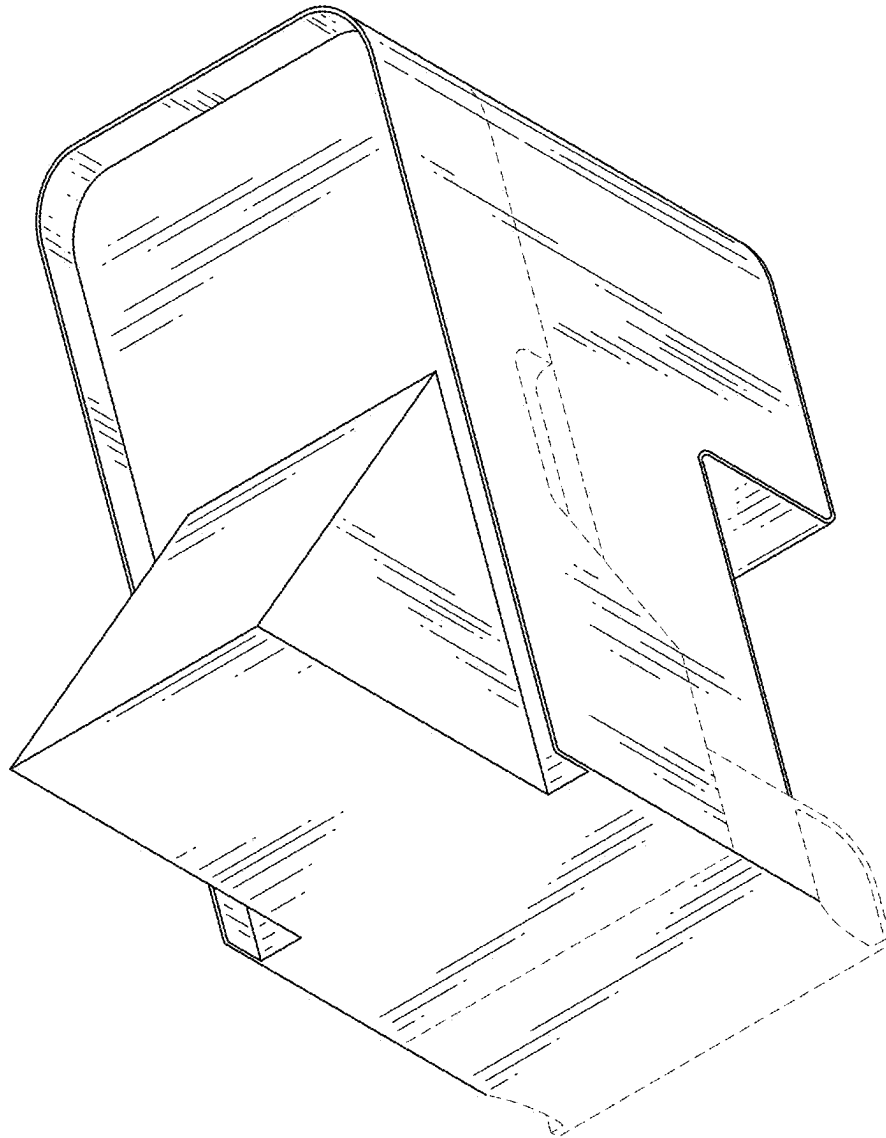


FIG.3

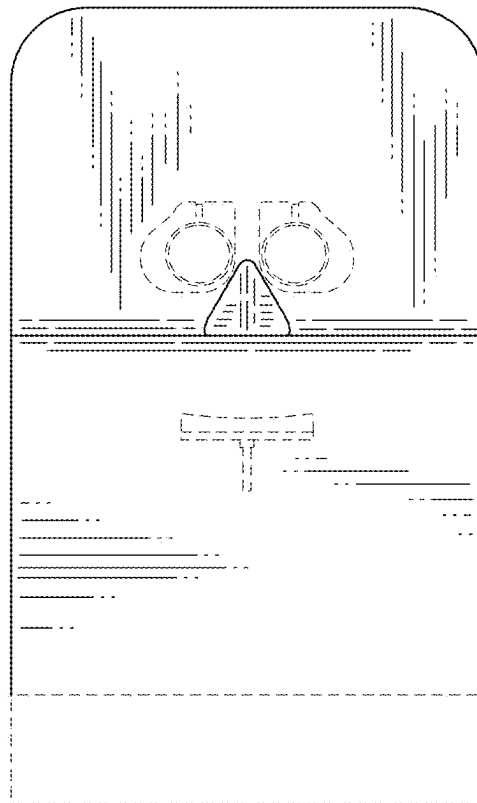


FIG.4

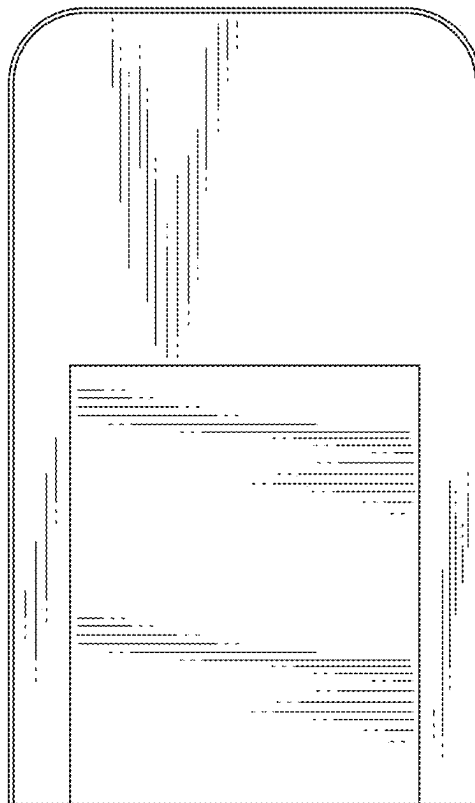


FIG.5

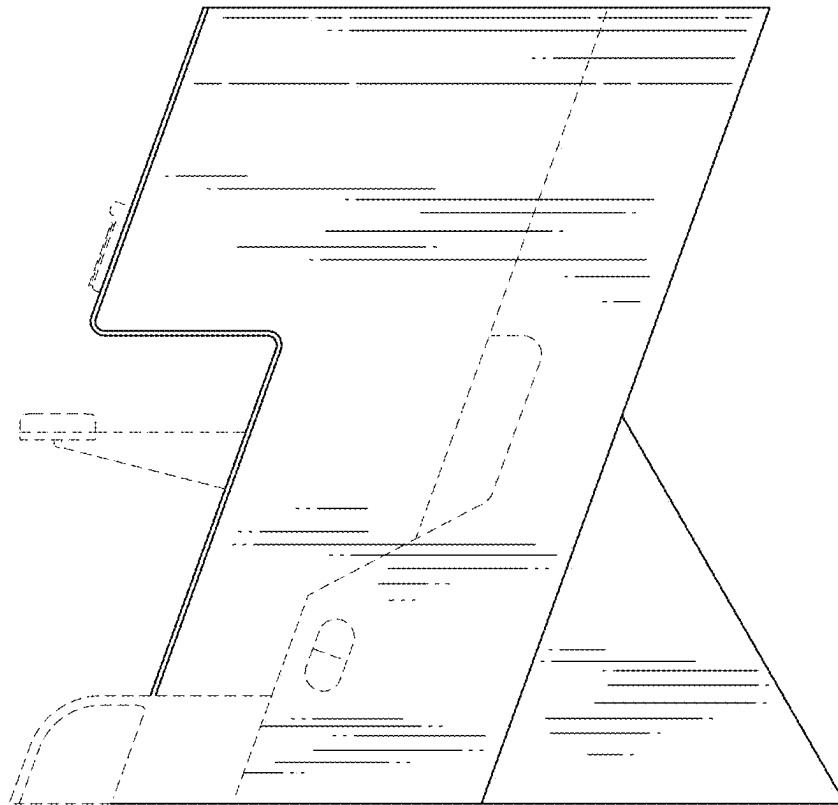


FIG.6

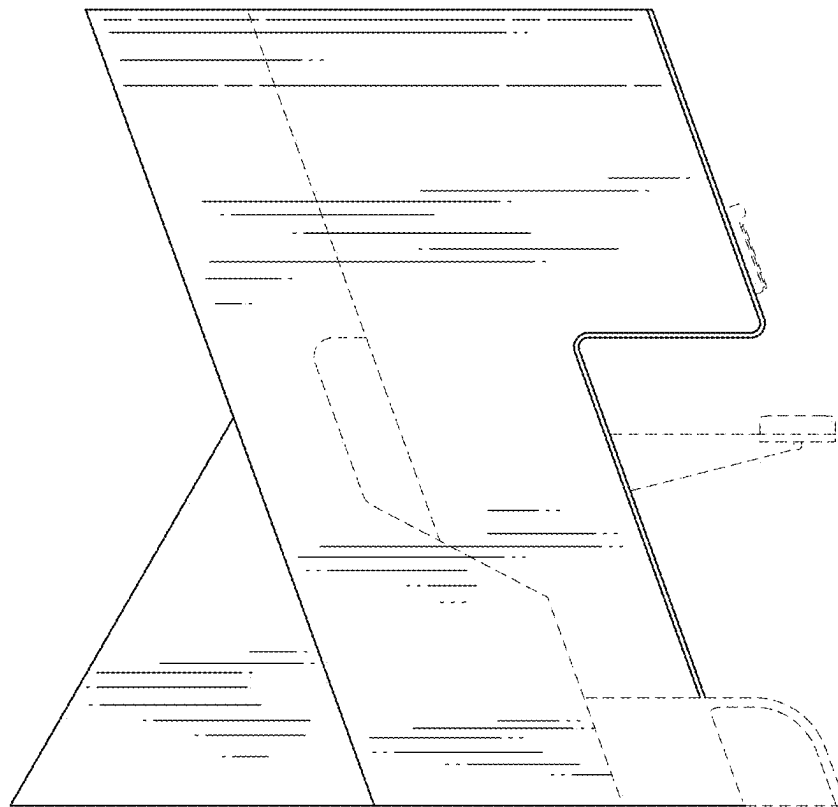


FIG.7

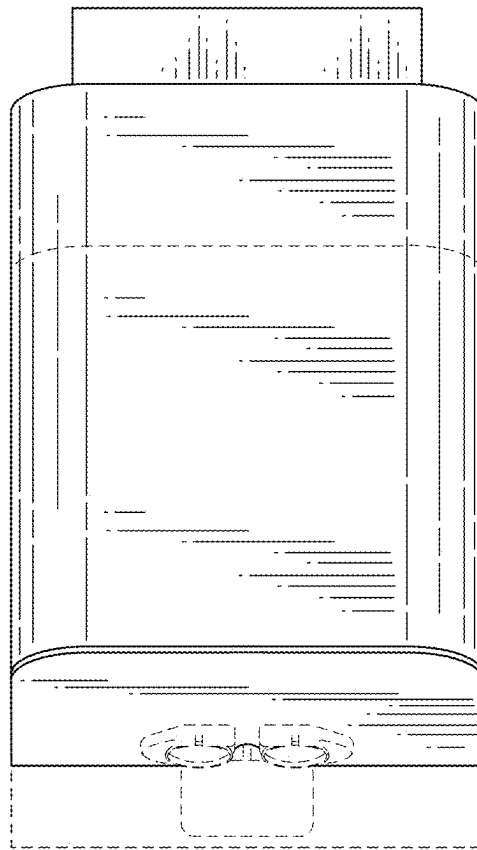


FIG.8

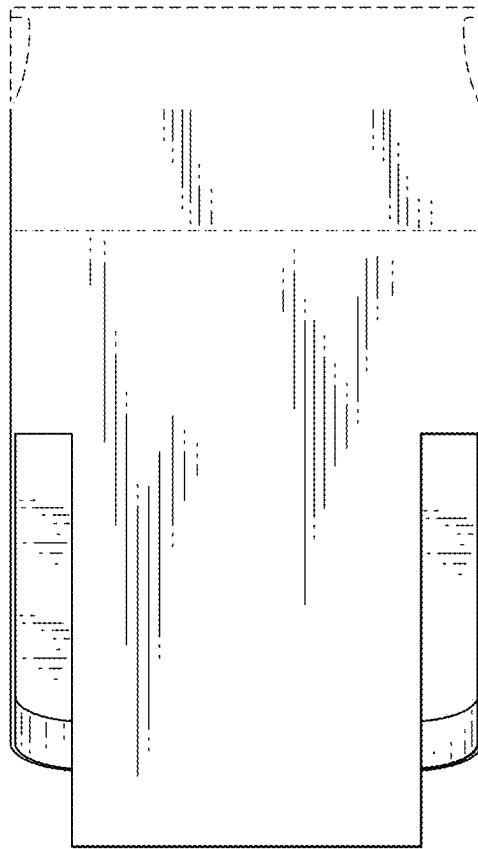


FIG.9